

Lever-Type Dial Indicators DIAL TEST INDICATORS

SMALL TOOL INSTRUMENTS
AND DATA MANAGEMENT



NEW
Products

Enhanced Durability, Sensitivity and Readability



Inspection

- The QR code is used by the factory to accurately match the inspection certificate to the test indicator.




Stylus length is marked on the dial face

- Stylus length is marked on the dial face to assist customers when ordering replacement styli.



Attachable limit hands

- Limit hands (optional) can be attached to the bezel, allowing easy identification of the upper and lower limits of tolerance.

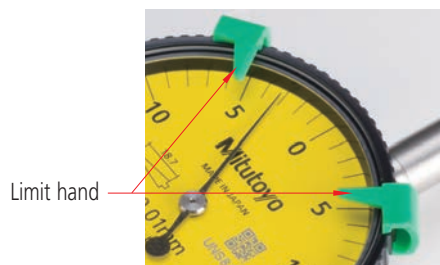

ø8/ø9.52 stem to fit dovetails is a standard accessory

- A ø8mm (ø0.315 in) plain stem (**21CAB104**) for the Metric models or a ø9.52mm (ø3/8 in) plain stem (**21CAB105**) for the Inch models that attaches to any dovetail on the frame is supplied as a standard accessory. Other sizes are available as optional accessories:

ø4mm (ø0.157 in) stem: **21CAB106**

ø6mm (ø0.236 in) stem: **21CAB103**


certificate provided

CERTIFICATE OF INSPECTION 検査成績書			
Product Name: DML Test Indicator	Serial No.: 1704085	Certificate No.: 4240170830	Temperature: 20°C (Standard temperature)
Scale: 0.01mm	Scale interval: 0.01mm	Measuring range: 0 to 8mm	Measuring range: 0 to 8mm
Model: 1704085			
Inspection results			
Item	Unit	Value	Remarks
1. Overall length (mm)	mm	15.2	One piece
2. Overall length (mm)	mm	11.2	First 2.5mm
3. Overall length (mm)	mm	9.4	First 2.5mm
4. Overall length (mm)	mm	0.61	First 2.5mm
5. Overall length (mm)	mm	0.45	First 2.5mm
6. Overall length (mm)	mm	0.37	First 2.5mm
7. Overall length (mm)	mm	0.37	First 2.5mm
8. Overall length (mm)	mm	0.37	First 2.5mm
9. Overall length (mm)	mm	0.37	First 2.5mm
10. Overall length (mm)	mm	0.37	First 2.5mm
11. Overall length (mm)	mm	0.37	First 2.5mm
12. Overall length (mm)	mm	0.37	First 2.5mm
13. Overall length (mm)	mm	0.37	First 2.5mm
14. Overall length (mm)	mm	0.37	First 2.5mm
15. Overall length (mm)	mm	0.37	First 2.5mm
16. Overall length (mm)	mm	0.37	First 2.5mm
17. Overall length (mm)	mm	0.37	First 2.5mm
18. Overall length (mm)	mm	0.37	First 2.5mm
19. Overall length (mm)	mm	0.37	First 2.5mm
20. Overall length (mm)	mm	0.37	First 2.5mm
21. Overall length (mm)	mm	0.37	First 2.5mm
22. Overall length (mm)	mm	0.37	First 2.5mm
23. Overall length (mm)	mm	0.37	First 2.5mm
24. Overall length (mm)	mm	0.37	First 2.5mm
25. Overall length (mm)	mm	0.37	First 2.5mm
26. Overall length (mm)	mm	0.37	First 2.5mm
27. Overall length (mm)	mm	0.37	First 2.5mm
28. Overall length (mm)	mm	0.37	First 2.5mm
29. Overall length (mm)	mm	0.37	First 2.5mm
30. Overall length (mm)	mm	0.37	First 2.5mm
31. Overall length (mm)	mm	0.37	First 2.5mm
32. Overall length (mm)	mm	0.37	First 2.5mm
33. Overall length (mm)	mm	0.37	First 2.5mm
34. Overall length (mm)	mm	0.37	First 2.5mm
35. Overall length (mm)	mm	0.37	First 2.5mm
36. Overall length (mm)	mm	0.37	First 2.5mm
37. Overall length (mm)	mm	0.37	First 2.5mm
38. Overall length (mm)	mm	0.37	First 2.5mm
39. Overall length (mm)	mm	0.37	First 2.5mm
40. Overall length (mm)	mm	0.37	First 2.5mm
41. Overall length (mm)	mm	0.37	First 2.5mm
42. Overall length (mm)	mm	0.37	First 2.5mm
43. Overall length (mm)	mm	0.37	First 2.5mm
44. Overall length (mm)	mm	0.37	First 2.5mm
45. Overall length (mm)	mm	0.37	First 2.5mm
46. Overall length (mm)	mm	0.37	First 2.5mm
47. Overall length (mm)	mm	0.37	First 2.5mm
48. Overall length (mm)	mm	0.37	First 2.5mm
49. Overall length (mm)	mm	0.37	First 2.5mm
50. Overall length (mm)	mm	0.37	First 2.5mm
51. Overall length (mm)	mm	0.37	First 2.5mm
52. Overall length (mm)	mm	0.37	First 2.5mm
53. Overall length (mm)	mm	0.37	First 2.5mm
54. Overall length (mm)	mm	0.37	First 2.5mm
55. Overall length (mm)	mm	0.37	First 2.5mm
56. Overall length (mm)	mm	0.37	First 2.5mm
57. Overall length (mm)	mm	0.37	First 2.5mm
58. Overall length (mm)	mm	0.37	First 2.5mm
59. Overall length (mm)	mm	0.37	First 2.5mm
60. Overall length (mm)	mm	0.37	First 2.5mm
61. Overall length (mm)	mm	0.37	First 2.5mm
62. Overall length (mm)	mm	0.37	First 2.5mm
63. Overall length (mm)	mm	0.37	First 2.5mm
64. Overall length (mm)	mm	0.37	First 2.5mm
65. Overall length (mm)	mm	0.37	First 2.5mm
66. Overall length (mm)	mm	0.37	First 2.5mm
67. Overall length (mm)	mm	0.37	First 2.5mm
68. Overall length (mm)	mm	0.37	First 2.5mm
69. Overall length (mm)	mm	0.37	First 2.5mm
70. Overall length (mm)	mm	0.37	First 2.5mm
71. Overall length (mm)	mm	0.37	First 2.5mm
72. Overall length (mm)	mm	0.37	First 2.5mm
73. Overall length (mm)	mm	0.37	First 2.5mm
74. Overall length (mm)	mm	0.37	First 2.5mm
75. Overall length (mm)	mm	0.37	First 2.5mm
76. Overall length (mm)	mm	0.37	First 2.5mm
77. Overall length (mm)	mm	0.37	First 2.5mm
78. Overall length (mm)	mm	0.37	First 2.5mm
79. Overall length (mm)	mm	0.37	First 2.5mm
80. Overall length (mm)	mm	0.37	First 2.5mm
81. Overall length (mm)	mm	0.37	First 2.5mm
82. Overall length (mm)	mm	0.37	First 2.5mm
83. Overall length (mm)	mm	0.37	First 2.5mm
84. Overall length (mm)	mm	0.37	First 2.5mm
85. Overall length (mm)	mm	0.37	First 2.5mm
86. Overall length (mm)	mm	0.37	First 2.5mm
87. Overall length (mm)	mm	0.37	First 2.5mm
88. Overall length (mm)	mm	0.37	First 2.5mm
89. Overall length (mm)	mm	0.37	First 2.5mm
90. Overall length (mm)	mm	0.37	First 2.5mm
91. Overall length (mm)	mm	0.37	First 2.5mm
92. Overall length (mm)	mm	0.37	First 2.5mm
93. Overall length (mm)	mm	0.37	First 2.5mm
94. Overall length (mm)	mm	0.37	First 2.5mm
95. Overall length (mm)	mm	0.37	First 2.5mm
96. Overall length (mm)	mm	0.37	First 2.5mm
97. Overall length (mm)	mm	0.37	First 2.5mm
98. Overall length (mm)	mm	0.37	First 2.5mm
99. Overall length (mm)	mm	0.37	First 2.5mm
100. Overall length (mm)	mm	0.37	First 2.5mm

Extended stylus length for 0.001mm, 0.002mm, and 0.0001" graduation models



- Longer styli for the most sensitive indicators allow access to difficult-to-measure features.

0.001mm graduation models: L2 now 15.2mm, was 11.2mm
 0.002mm graduation models: L2 now 11.2mm, was 9.4mm
 0.0001 in graduation models: L2 now 0.61 in, was 0.45 in



Ruby ball-tipped stylus added

- A ruby tip has wear-resistance several times greater than a carbide tip and, since it is nonconductive, it can be used safely on an electrical discharge machine.

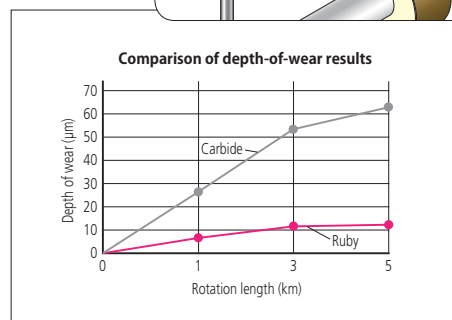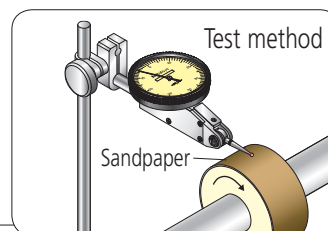

Enhanced Durability, Sensitivity and Readability



Crystal for readability

- Glare-free flat crystal face allows easy reading of graduations.



Conventional

New

Prevents dust and oil from penetrating the dial face


- The O-ring seal on the bezel provides smooth rotation and prevents dust and oil from penetrating the dial face.

Bonded bezel and crystal

- Bonding the bezel and crystal eliminates a gap for cutting fluid or oil to penetrate the dial face.

Prevents bezel detachment

- A flange prevents the bezel from unintentionally being removed during handling.

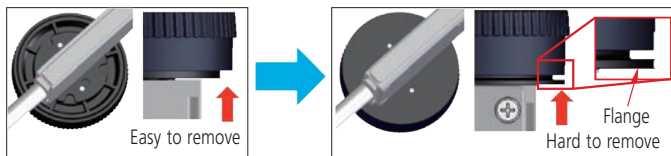

Conventional


New

Maintain trackability

- The ability of the indicator to track small changes in displacement deteriorates with prolonged use due to minute changes in clearance between the gears. Redesigned mounting for the gears enables the ability to maintain good trackability.

Improved readability

- Using universal fonts, changing dial face color and reviewing the relationship between pointer and scale marks have drastically improved readability.

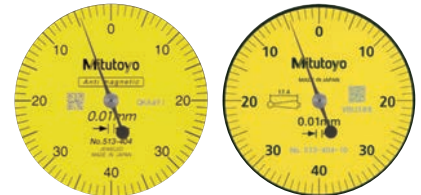

Conventional

New



Parts



Choice of dial position

Four models are available, each with a different orientation of the dial to allow the best visibility in any situation.

- Horizontal (standard model) - dial is on top of the frame.
- Vertical: dial is on the end of the frame.
- Horizontal (20° tilted face): dial is on top of the frame but tilted 20°.
- Parallel: dial is on the side of the frame.




Multi-layer coatings on the crystal


- Hard, antifouling and non-glare coatings on the crystal inhibit scratches, contamination and glare on the surface.

Improved stylus bearing


- The conventional method of mounting the stylus pivot bearing screw in the frame is prone to loosen with prolonged use. A unique sub-plate structure has been incorporated in all models to eliminate this issue.



Stylus bearing screw held in frame.



Stylus bearing screw held in sub-plate.



Indicator trackability depends on maintaining gear-train stability


Set Configuration

Inch

Full set



Basic set

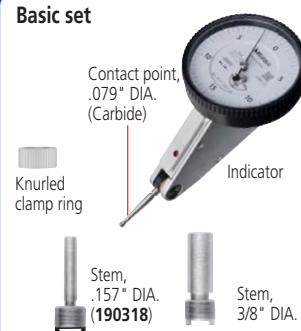

T set

E set

Metric

Full set



Plus set



Basic set



T set

A set

C set
(ø 6 Stem)

E set

H set
(ø 6 Stem)




Horizontal (Standard model)

Metric Wide variations of models conform to the required accuracy, range and surface of workpieces.



513-424-10

Contact point No. 137557



Graduation: 0.01mm
Range: 0.5mm

513-424-10E/513-424-10A/
513-424-10T

- Standard
- Double scale spacing
- Carbide contact point (Anti-magnet)



513-414-10

Contact point No. 131324



Graduation: 0.01mm
Range: 0.5mm

513-414-10E/513-414-10A/
513-414-10T

- Long stylus
- Carbide contact point (Anti-magnet)
- Double scale spacing



513-478-10

Contact point No. 21CZA210



Graduation: 0.01mm
Range: 0.5mm

513-478-10E

- Ruby contact point (non-magnet)
- Standard
- Double scale spacing



513-474-10

Contact point No. 21CZA201



Graduation: 0.01mm
Range: 0.8mm

513-474-10E

- Ruby contact point (non-magnet)
- Standard



513-466-10

Contact point No. 137557



Graduation: 0.01mm
Range: 0.5mm

513-466-10E

- Small face diameter
- Double scale spacing
- Compact
- Carbide contact point (Anti-magnet)



513-464-10

Contact point No. 103006



Graduation: 0.01mm
Range: 0.8mm


513-464-10E

- Small face diameter
- Compact
- Carbide contact point (Anti-magnet)



513-404-10

Contact point No. 103006



Graduation: 0.01mm
Range: 0.8mm

513-404-10E/513-404-10A/
513-404-10T/513-404-10C

- Standard
- Carbide contact point (Anti-magnet)



513-415-10

Contact point No. 136013



Graduation: 0.01mm
Range: 1.0mm

513-415-10E/513-415-10A/
513-415-10T

- Long stylus
- Carbide contact point (Anti-magnet)



513-477-10

Contact point No. 21CZA211



Graduation: 0.01mm
Range: 1.0mm

513-477-10E

Ruby contact point (non-magnet)

Long stylus



513-475-10

Contact point No. 21CZB068



Graduation: 0.002mm
Range: 0.2mm

513-475-10E

Ruby contact point (non-magnet)

Standard



513-426-10

Contact point No. 137557



Graduation: 0.01mm
Range: 1.5mm

513-426-10E/513-426-10A

With revolution counter

Double scale spacing

Carbide contact point (Anti-magnet)



513-425-10

Contact point No. 103011



Graduation: 0.002mm
Range: 0.6mm

513-425-10E/513-425-10A


With revolution counter

Carbide contact point (Anti-magnet)



513-405-10

Contact point No. 103011



Graduation: 0.002mm
Range: 0.2mm

513-405-10E/513-405-10A/
513-405-10T


Standard

Carbide contact point (Anti-magnet)



513-465-10

Contact point No. 103011



Graduation: 0.002mm
Range: 0.2mm

513-465-10E

Small face diameter

Compact

Carbide contact point (Anti-magnet)



513-471-10

Contact point No. 21CZA209



Graduation: 0.001mm
Range: 0.14mm

513-471-10E

Ruby contact point (non-magnet)

High accuracy



513-401-10

Contact point No. 103010



Graduation: 0.001mm
Range: 0.14mm

513-401-10E

High accuracy

Carbide contact point (Anti-magnet)



Horizontal (Standard model)

Inch



513-402-10

Contact point No. 133195



Graduation: 0.0005 in
Range: 0.03 in

513-402-10E/513-402-10T

- Standard
- Carbide contact point (Anti-magnet)



513-462-10

Contact point No. 133195



Graduation: 0.0005 in
Range: 0.03 in

513-462-10E

- Compact
- Carbide contact point (Anti-magnet)



513-472-10

Contact point No. 21CZA204



Graduation: 0.0005 in
Range: 0.03 in

513-472-10E

- Standard
- Ruby contact point (non-magnet)



513-403-10

Contact point No. 21CZB064



Graduation: 0.0001 in
Range: 0.008 in

513-403-10E/513-403-10T

- Standard
- Anti-magnet (non-magnet)



513-412-10

Contact point No. 136290



Graduation: 0.0005 in
Range: 0.03 in

513-412-10E/513-412-10T

- Long stylus
- Carbide contact point (Anti-magnet)



513-473-10

Contact point No. 21CZB112



Graduation: 0.0001 in
Range: 0.008 in

513-473-10E

- Standard
- Ruby contact point (non-magnet)



512-479-10

Contact point No. 21CZA214



Graduation: 0.0005 in
Range: 0.03 in

512-479-10E

- Long stylus
- Ruby contact point (non-magnet)



513-463-10

Contact point No. 21CZB064



Graduation: 0.0001 in
Range: 0.008 in

513-463-10E

- Compact
- Carbide contact point (Anti-magnet)

Metric/Inch



513-409-10

Contact point No. 103011



Graduation: 0.002mm/0.0001 in
Range: 0.2mm/0.0076 in

513-409-10E/513-409-10T


Carbide contact point (Anti-magnet)

Inch/Metric



513-406-10

Contact point No. 133195



Graduation: 0.0005 in/0.01mm
Range: 0.03 in/0.7mm


513-406-10E/513-406-10T

Carbide contact point (Anti-magnet)

DIMENSIONS

Vertical


Unit: mm

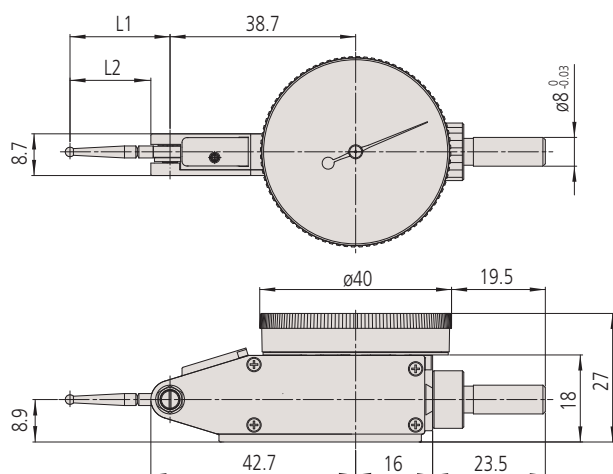

Type	Order No.	L1	L2
Vertical	513-401-10E	14.7	11.2
	513-471-10E		
	513-405-10E/A/T		
	513-415-10E/A		
	513-475-10E	18.7	15.2
	513-404-10E/A/T		
	513-474-10E		
	513-424-10E/A/T		
	513-426-10E/A	22.2	18.7
	513-478-10E		
	513-414-10E/A/T	37.4	33.9
	513-415-10E/A/T	44.5	41.0
	513-477-10E		

Compact

Unit: mm

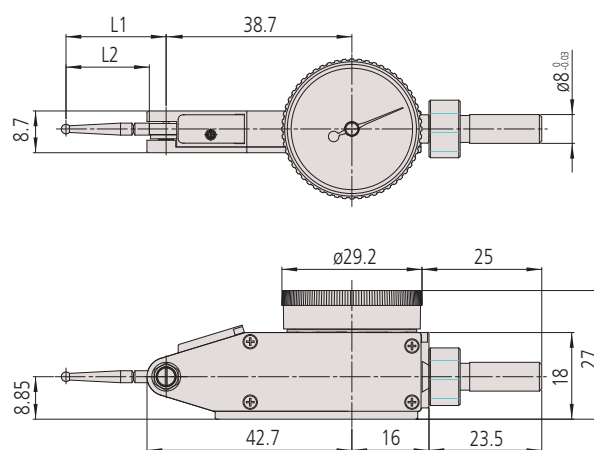

Type	Order No.	L1	L2
Compact	513-465-10E	18.7	15.2
	513-464-10E	20.9	17.4
	513-466-10E	22.2	18.7



Horizontal (Standard model)

SPECIFICATIONS

Metric

Order No.			Graduation	Range	Dial reading	Indication accuracy				Mass	Measuring force	 High accuracy	 With revolution counter	 Long stylus	 Standard	 Double scale spacing	 Compact	 Carbide contact point (Anti-magnet)	 Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	10 scale divisions	Hysteresis	Repeatability										
513-424-10E	513-424-10A	513-424-10T	0.01 mm	0.5 mm	0-25-0	6 μm	4 μm	3 μm	45g	0.3N or less									
513-478-10E	—	—				6 μm			41g	0.3N or less									
513-466-10E	—	—		0.8 mm	0-40-0	9 μm	4 μm	45g	0.2N or less										
513-404-10E	513-404-10A	513-404-10T				9 μm			0.2N or less										
513-414-10E	513-414-10A	513-414-10T		0.5 mm	0-25-0	10 μm	5 μm	3 μm	45g	0.2N or less									
513-474-10E	—	—				10 μm			0.3N or less										
513-464-10E	—	—		0.8 mm	0-40-0	9 μm	4 μm	41g	0.3N or less										
513-415-10E	513-415-10A	513-415-10T				9 μm			0.2N or less										
513-477-10E	—	—	0.01 mm	1.0 mm	0-50-0	10 μm	5 μm		45g	0.2N or less									
513-426-10E	513-426-10A	—				16 μm			0.4N or less										
513-405-10E	513-405-10A	513-405-10T	0.002 mm	0.2 mm	0-100-0	2 μm	3 μm	1 μm	45g	0.3N or less									
513-471-10E	—	—	0.001 mm	0.14 mm	0-70-0					4 μm	0.3N or less								
513-475-10E	—	—	0.002 mm	0.2 mm	0-100-0		7 μm		4 μm	0.4N or less									
513-425-10E	513-425-10A	—		0.6 mm						0.4N or less									
513-465-10E	—	—	0.001 mm	0.2 mm	0-70-0		4 μm		3 μm	41g	0.3N or less								
513-401-10E	—	—								0.14 mm	0.3N or less								

Inch

Order No.			Graduation	Range	Dial reading	Indication accuracy			Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				One rev.	Hysteresis	Repeatability										
513-402-10E	—	513-402-10T	0.0005 in	0.03 in	0-15-0	±0.0005 in	0.0002 in	0.0002 in	45g	0.3N or less								
513-472-10E	—	—								0.2N or less								
513-412-10E	—	513-412-10T								0.2N or less								
513-479-10E	—	—								41g	0.3N or less							
513-462-10E	—	—	0.0001 in	0.008 in	0-4-0	±0.0001 in	0.0001 in	0.00004 in	45g	0.3N or less								
513-403-10E	—	513-403-10T							41g	0.3N or less								
513-473-10E	—	—							41g	0.3N or less								

Metric/Inch

Order No.			Graduation	Range	Dial reading	Indication accuracy				Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	10 scale divisions	Hysteresis	Repeatability										
513-409-10E	—	513-409-10T	0.002mm / 0.0001 in	0.2mm / 0.0076 in	0-10-0 / 0-35-0	4μm	2μm	3μm	1μm	45g	0.3N or less								

Inch/Metric

Order No.			Graduation	Range	Dial reading	Indication accuracy			Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	Hysteresis	Repeatability										
513-406-10E	—	513-406-10T	0.0005 in / 0.01mm	0.03 in / 0.7mm	0-15-0 / 0-35-0	±0.0005 in	0.0002 in	0.0002 in	45g	0.3N or less								


* Stem with ø6 dovetail groove is not included in the mass.

* Be sure to perform calibration with reference gage, etc. after changing the contact point. The inside parts may be damaged when the contact point is changed due to the breakage. In the case the of the significant deterioration during the operation, repair is required.



Parallel (The scale can be read from the front, with the contact point pivoting in a plane parallel to that of the dial face.)

Metric




513-484-10E/513-484-10A/
513-484-10T

Carbide contact point (Anti-magnet)



513-486-10E

Double scale spacing
 Carbide contact point (Anti-magnet)



513-485-10E

Carbide contact point (Anti-magnet)



513-482-10A/513-482-10T

Carbide contact point (Anti-magnet)

SPECIFICATIONS

Metric

Order No.			Graduation	Range	Dial reading	Indication accuracy				Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	10 scale divisions	Hysteresis	Repeatability										
513-484-10E	513-484-10A	513-484-10T	0.01mm	0.8mm	0-40-0	9μm	5μm	4μm	3μm	53g	0.3N or less								
513-485-10E	-	-	0.002mm	0.2mm	0-100-0	4μm	2μm	3μm	1μm										
513-486-10E	-	-	0.01mm	0.5mm	0-25-0	6μm	5μm	4μm	3μm							✓		✓	

Inch


Order No.			Graduation	Range	Dial reading	Indication accuracy			Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	Hysteresis	Repeatability										
-	513-482-10A	513-482-10T	0.0005 in	0.03 in	0-15-0	±0.0005 in	0.0002 in	0.0002 in	53g	0.3N or less							✓	

* Stem with ø6 dovetail groove is not included in the mass.

* Be sure to perform calibration with reference gage, etc. after changing the contact point. The inside parts may be damaged when the contact point is changed due to the breakage. In the case the of the significant deterioration during the operation, repair is required.

DIMENSIONS

* No dovetail in the back.

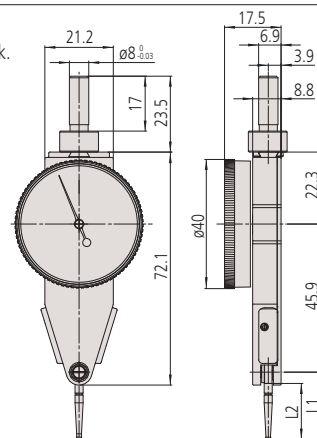

Unit: mm

Order No.	L1	L2
513-484-10E	20.9	17.4
513-485-10E	18.7	15.2
513-486-10E	22.2	18.7



Vertical (Best suited for centering holes under the spindle of a machine tool.)

Metric



513-454-10

Contact point No. 103006



Graduation: 0.01mm
Range: 0.8mm


513-454-10E/513-454-10A/
513-454-10T

Carbide contact
point (Anti-magnet)



513-455-10

Contact point No. 103011



Graduation: 0.002mm
Range: 0.2mm

513-455-10E/513-455-10A/
513-455-10T

Carbide contact
point (Anti-magnet)



513-456-10

Contact point No. 137557



Graduation: 0.01mm
Range: 0.5mm

513-456-10E

Double scale spacing
 Carbide contact
point (Anti-magnet)

Inch



513-452-10

Contact point No. 133195



Graduation: 0.0005 in
Range: 0.03 in

513-452-10E/513-452-10T

Carbide contact
point (Anti-magnet)



513-453-10

Contact point No. 21CZB064



Graduation: 0.0001 in
Range: 0.008 in

513-453-10E/513-453-10T

Carbide contact
point (Anti-magnet)

SPECIFICATIONS

Metric

Order No.			Graduation	Range	Dial reading	Indication accuracy				Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	10 scale divisions	Hysteresis	Repeatability										
513-454-10E	513-454-10A	513-454-10T	0.01mm	0.8mm	0-40-0	9μm	5μm	4μm	3μm	46g	0.3N or less	☒	☒	☒	☒	☒	☒	☒	☒
513-455-10E	513-455-10A	513-455-10T	0.002mm	0.2mm	0-100-0	4μm	2μm	3μm	1μm			☐	☐	☐	☐	☐	☐	☒	☒
513-456-10E	—	—	0.01mm	0.5mm	0-25-0	6μm	5μm	4μm	3μm			☐	☐	☐	☒	☐	☐	☒	☐

Inch


Order No.			Graduation	Range	Dial reading	Indication accuracy			Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	Hysteresis	Repeatability										
513-452-10E	—	513-452-10T	0.0005 in	0.03 in	0-15-0	±0.0005 in	0.0002 in	0.0002 in	46g	0.3N or less	☐	☒	☒	☒	☒	☒	☒	☒
513-453-10E	—	513-453-10T	0.0001 in	0.008 in	0-4-0	±0.0001 in	0.0001 in	0.00004 in			☐	☐	☐	☐	☐	☐	☒	☐

* Stem with ø6 dovetail groove is not included in the mass.

* Be sure to perform calibration with reference gage, etc. after changing the contact point. The inside parts may be damaged when the contact point is changed due to the breakage. In the case the of the significant deterioration during the operation, repair is required.

DIMENSIONS

Unit: mm

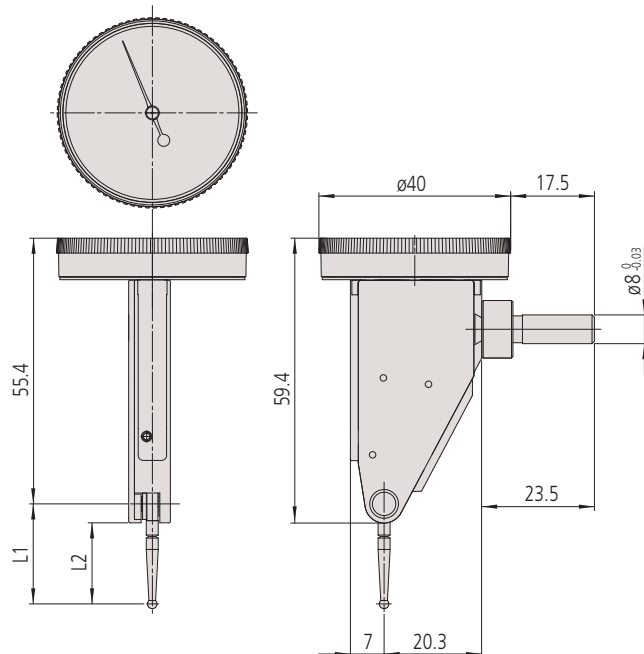

Order No.	L1	L2
513-454-10E	20.9	17.4
513-455-10E	18.7	15.2
513-456-10E	22.2	18.7




Horizontal (20° Tilted Face) (Dial face inclined 20°, compared with the vertical type.)

Metric



513-444-10

Contact point No. 103006



Graduation: 0.01mm
Range: 1.6mm

513-444-10E/513-444-10A/
513-444-10T

- ☒ With revolution counter
- ☒ Carbide contact point (Anti-magnet)



513-445-10

Contact point No. 103011



Graduation: 0.02mm
Range: 0.4mm

513-445-10E/513-445-10A/
513-445-10T

- ☒ With revolution counter
- ☒ Carbide contact point (Anti-magnet)

Inch



513-442-10

Contact point No. 133195



Graduation: 0.0005 in
Range: 0.06 in

513-442-10A/513-442-10T

- ☒ With revolution counter
- ☒ Carbide contact point (Anti-magnet)



513-442-16

Contact point No. 133195



Graduation: 0.0005 in
Range: 0.06 in

513-442-16A/513-442-16T

- ☒ With revolution counter
- ☒ Carbide contact point (Anti-magnet)



513-446-10

Contact point No. 136290



Graduation: 0.0005 in
Range: 0.06 in

513-446-10A/513-446-10T

- ☒ With revolution counter
- ☒ Long stylus
- ☒ Carbide contact point (Anti-magnet)



513-446-16

Contact point No. 136290



Graduation: 0.0005 in
Range: 0.06 in

513-446-16A/513-446-16T

- ☒ With revolution counter
- ☒ Long stylus
- ☒ Carbide contact point (Anti-magnet)



513-443-10

Contact point No. 21CZB064



Graduation: 0.0001 in
Range: 0.016 in

513-443-10A/513-443-10T

- ☒ With revolution counter
- ☒ Carbide contact point (Anti-magnet)



513-443-16

Contact point No. 21CZB064



Graduation: 0.0001 in
Range: 0.016 in

513-443-16A/513-443-16T

- ☒ With revolution counter
- ☒ Carbide contact point (Anti-magnet)

SPECIFICATIONS

Metric

Order No.			Graduation	Range	Dial reading	Indication accuracy				Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	10 scale divisions	Hysteresis	Repeatability										
513-444-10E	513-444-10A	513-444-10T	0.01mm	1.6mm	0-40-0	16μm	5μm	5μm	3μm	48g	0.3N or less		✓					✓	
513-445-10E	513-445-10A	513-445-10T	0.002mm	0.4mm	0-100-0	6μm	2μm	4μm	1μm										

Inch


Order No.			Graduation	Range	Dial reading	Indication accuracy			Mass	Measuring force	High accuracy	With revolution counter	Long stylus	Standard	Double scale spacing	Compact	Carbide contact point (Anti-magnet)	Ruby contact point (non-magnet)
Basic set	Plus set	Full set				Measuring range	Hysteresis	Repeatability										
–	513-442-10A	513-442-10T	0.0005 in	0.06 in	0-15-0	±0.0005 in	0.0002 in	0.0002 in	48g	0.3N or less		✓					✓	
–	513-442-16A	513-442-16T								0.2N or less		✓					✓	
–	513-446-10A	513-446-10T										✓	✓				✓	
–	513-446-16A	513-446-16T										✓	✓				✓	
–	513-443-10A	513-443-10T	0.0001 in	0.016 in	0-4-0	±0.0002 in	0.0001 in	0.00004 in		0.3N or less		✓					✓	
–	513-443-16A	513-443-16T										✓					✓	

* Stem with ø6 dovetail groove is not included in the mass.

* Be sure to perform calibration with reference gage, etc. after changing the contact point. The inside parts may be damaged when the contact point is changed due to the breakage. In the case of the significant deterioration during the operation, repair is required.


DIMENSIONS

Unit: mm

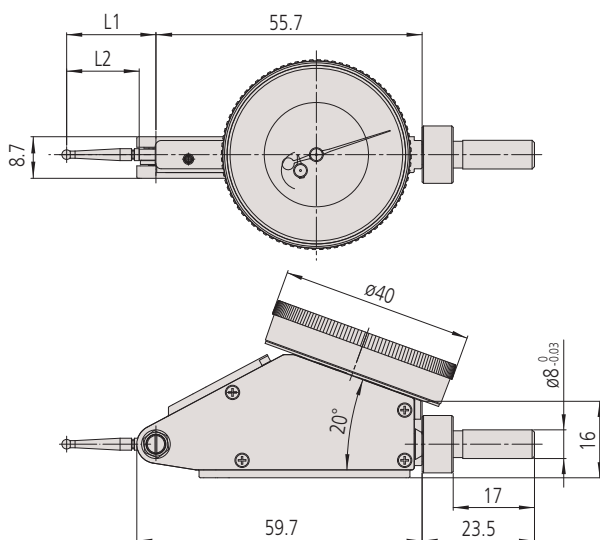

Order No.	L1	L2
513-445-10E	18.7	15.2
513-444-10E	20.9	17.4

Refer to MEASURING INSTRUMENTS CATALOG No. US-1004 for the accessories such as styli, stems with dovetail, holding bars, etc.

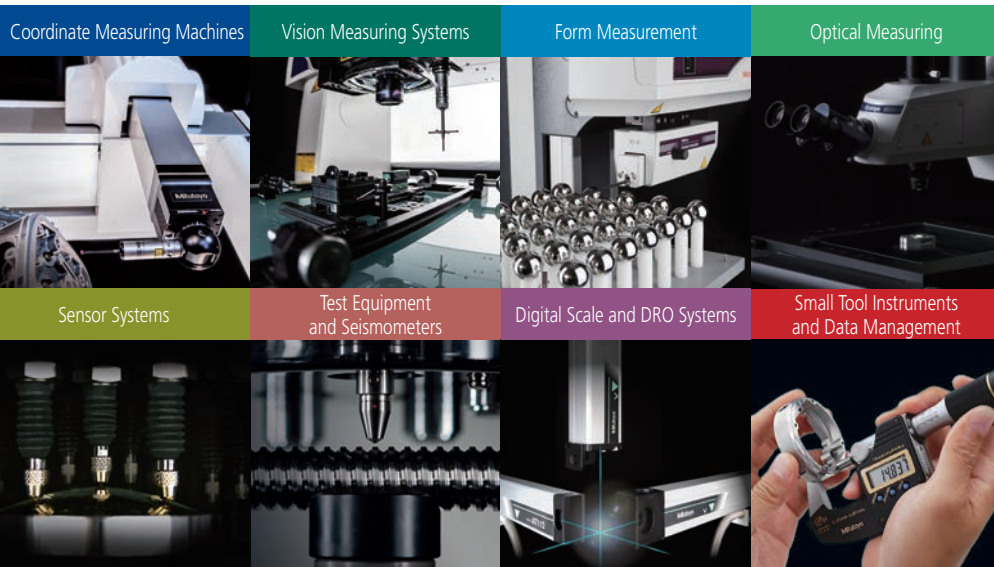

**Whatever your challenges are,
Mitutoyo supports you from start to finish.**

Mitutoyo is not only a manufacturer of top-quality measuring products but one that also offers qualified support for the lifetime of the equipment, backed by comprehensive services that ensure your staff can make the very best use of the investment.

Apart from the basics of calibration and repair, Mitutoyo offers product and metrology training, as well as IT support for the sophisticated software used in modern measuring technology. We can also design, build, test and deliver measuring solutions and even, if deemed cost-effective, take your critical measurement challenges in-house on a sub-contract basis.



**Find additional product literature
and our product catalog**

www.mitutoyo.com

Note: All information regarding our products, and in particular the illustrations, drawings, dimensional and performance data contained in this printed matter as well as other technical data are to be regarded as approximate average values. We therefore reserve the right to make changes to the corresponding designs. The stated standards, similar technical regulations, descriptions and illustrations of the products were valid at the time of printing. In addition, the latest applicable version of our General Trading Conditions will apply. Only quotations submitted by ourselves may be regarded as definitive. Specifications are subject to change without notice.

Mitutoyo products are subject to US Export Administration Regulations (EAR). Re-export or relocation of our products may require prior approval by an appropriate governing authority.

Trademarks and Registrations

Designations used by companies to distinguish their products are often claimed as trademarks. In all instances where Mitutoyo America Corporation is aware of a claim, the product names appear in initial capital or all capital letters. The appropriate companies should be contacted for more complete trademark and registration information.

Mitutoyo

Mitutoyo America Corporation

www.mitutoyo.com

One Number to Serve You Better

1-888-MITUTOYO (1-888-648-8869)

M³ Solution Centers:

Aurora, Illinois (Headquarters)
Boston, Massachusetts
Huntersville, North Carolina
Mason, Ohio
Plymouth, Michigan
City of Industry, California
Birmingham, Alabama
Renton, Washington
Houston, Texas