



Agilent Technologies
Low-Profile
Modular Power System
Series N6700

Service Guide



Agilent Technologies

Legal Notices

© Agilent Technologies, Inc. 2006 - 2010

No part of this document may be photocopied, reproduced, or translated to another language without the prior agreement and written consent of Agilent Technologies, Inc. as governed by United States and international copyright laws.

Warranty

The material contained in this document is provided "as is," and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Manual Editions

Manual Part Number: 5969-2938
Fifth Edition, October, 2010
Printed in Malaysia.

Reprints of this manual containing minor corrections and updates may have the same printing date. Revised editions are identified by a new printing date.

Waste Electrical and Electronic Equipment (WEEE) Directive 2002/96/EC

This product complies with the WEEE Directive 2002/96/EC) marketing requirement. The affixed product label (see below) indicates that you must not discard this electrical/electronic product in domestic household waste.

Product Category: With reference to the equipment types in the WEEE directive Annex 1, this product is classified as "Monitoring and Control instrumentation" product.

Do not dispose in domestic household waste.

To return unwanted products, contact our local Agilent office, or see www.agilent.com/environment/product for more information.



Certification

Agilent Technologies certifies that this product met its published specifications at time of shipment from the factory. Agilent Technologies further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology, to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

Exclusive Remedies

THE REMEDIES PROVIDED HEREIN ARE THE CUSTOMER'S SOLE AND EXCLUSIVE REMEDIES. AGILENT TECHNOLOGIES SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

Assistance

This product comes with the standard product warranty. Warranty options, extended support contacts, product maintenance agreements and customer assistance agreements are also available. Contact your nearest Agilent Technologies Sales and Service office for further information on Agilent Technologies' full line of Support Programs.

Technologies Licenses

The hardware and or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

U.S. Government Restricted Rights

Software and technical data rights granted to the federal government include only those rights customarily provided to end user customers. Agilent provides this customary commercial license in Software and technical data pursuant to FAR 12.211 (Technical Data) and 12.212 (Computer Software) and, for the Department of Defense, DFARS 252.227-7015 (Technical Data – Commercial Items) and DFARS 227.7202-3 (Rights in Commercial Computer Software or Computer Software Documentation).

Trademarks

Microsoft and Windows are U.S. registered trademarks of Microsoft Corporation.

Safety Notices

The following general safety precautions must be observed during all phases of operation of this instrument. Failure to comply with these precautions or with specific warnings or instructions elsewhere in this manual violates safety standards of design, manufacture, and intended use of the instrument. Agilent Technologies assumes no liability for the customer's failure to comply with these requirements.

General

Do not use this product in any manner not specified by the manufacturer. The protective features of this product may be impaired if it is used in a manner not specified in the operation instructions.

Before Applying Power

Verify that all safety precautions are taken. Make all connections to the unit before applying power. Note the instrument's external markings described under "Safety Symbols"

Ground the Instrument

This product is a Safety Class 1 instrument (provided with a protective earth terminal). To minimize shock hazard, the instrument chassis and cover must be connected to an electrical ground. The instrument must be connected to the ac power mains through a grounded power cable, with the ground wire firmly connected to an electrical ground (safety ground) at the power outlet. Any interruption of the protective (grounding) conductor or disconnection of the protective earth terminal will cause a potential shock hazard that could result in personal injury.

Fuses

The instrument contains an internal fuse, which is not customer accessible.

Do Not Operate in an Explosive Atmosphere

Do not operate the instrument in the presence of flammable gases or fumes.

Do Not Remove the Instrument Cover

Only qualified, service-trained personnel who are aware of the hazards involved should remove instrument covers. Always disconnect the power cable and any external circuits before removing the instrument cover.

Do Not Modify the Instrument

Do not install substitute parts or perform any unauthorized modification to the product. Return the product to an Agilent Sales and Service Office for service and repair to ensure that safety features are maintained.

In Case of Damage

Instruments that appear damaged or defective should be made inoperative and secured against unintended operation until they can be repaired by qualified service personnel.

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

WARNING


A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

Safety Symbols

	Direct current
	Alternating current
	Both direct and alternating current
	Three phase alternating current
	Earth (ground) terminal
	Protective earth ground terminal.
	Frame or chassis terminal
	Terminal is at earth potential.
	Neutral conductor on permanently installed equipment
	Line conductor on permanently installed equipment.
	On supply
	Off supply
	Standby supply. Unit is not completely disconnected from ac mains when switch is off
	In position of a bi-stable push switch
	Out position of a bi-stable push switch
	Caution, risk of electric shock
	Caution, hot surface
	Caution, refer to accompanying description

Contents

1	Introduction.....	5
	Returning an Instrument	6
	Instrument Identification.....	6
	Firmware Upgrade	7
2	Performance Verification	9
	Verification Description	9
	Verification Procedure	13
	Test Record Forms	13
3	Calibration.....	37
	Calibration Description	38
	Calibration Procedure	39
4	Disassembly.....	71
	 Electrostatic Discharge (ESD) Precautions.....	72
	Disassembly Procedures	72
	Installing a Redundant Ground for 400 Hz Operation	77
5	Troubleshooting.....	79
	Preliminary Checkout.....	80
	Overall Troubleshooting	81
	Front Panel Troubleshooting	84
	Bias Board Troubleshooting.....	84
	Backplane Board Troubleshooting	85
	Calibration and Passwords	86
	Initialization	86
6	Replaceable Parts	87
	Parts List.....	88
	Parts Location Diagrams	89
Appendix A	Error Messages	91
	Displaying Error Messages	92
	Error List.....	92
Appendix B	Backdating.....	97
	Firmware Differences.....	98
	Index.....	103

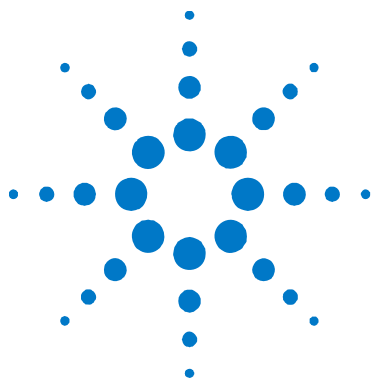

1

Introduction

Returning an Instrument	6
Instrument Identification	6
Firmware Upgrade	7

This manual discusses the troubleshooting procedures for the N6700B, N6701A, and N6702A MPS mainframes. Troubleshooting procedures are provided to isolate defective assemblies. These procedures do not troubleshoot to the component level.

No procedures are provided for troubleshooting individual modules - other than identifying if a specific module is defective. If you have a defective module, you can return it to Agilent Technologies for repair or replacement. Refer to the following note.

NOTE

You can contact Agilent Technologies at one of the following telephone numbers for warranty, service, or technical support information.

In the United States: (800) 829-4444

In Europe: 31 20 547 2111

In Japan: 0120-421-345

Or use our Web link for information on contacting Agilent in your country or specific location: www.agilent.com/find/assist

Or contact your Agilent Technologies Representative.

The web contains the most up to date version of the manuals. Go to <http://www.agilent.com/find/N6700> to get the latest version of the manuals.

Returning an Instrument

Before returning your instrument to Agilent Technologies for service or repair, perform the “Preliminary Checkout” procedures in the beginning of chapter 4.

Warranty Repair

If your instrument fails during the warranty period, Agilent Technologies will replace or repair it free of charge. After your warranty expires, Agilent Technologies will replace or repair it at a competitive price. The standard repair process is “whole unit exchange”. The replacement units are fully refurbished and are shipped with new calibration certificates.

Contact your nearest Agilent Technologies Service Center. They will arrange to have your instrument repaired or replaced.

Repackaging for Shipment

If the unit is to be shipped to Agilent Technologies for service or repair, be sure to:

- Attach a tag to the unit identifying the owner and indicating the required service or repair. Include the model and serial number.
- Place the unit in its original container with the appropriate packaging material and secure the container with strong tape or metal bands.

If the original shipping container is not available, place your unit in a container that will ensure at least 4 inches of compressible packaging material around all sides for the instrument. Use static-free packaging materials to avoid additional damage to your unit.

Agilent Technologies suggests that you always insure shipments.

Instrument Identification

Serial Number

Agilent N6700 MPS mainframes are identified by the serial number located on the interface cover.

The serial number consists of a 10-character number (e.g. MY24D00013) located on the label on the top of the interface board. The first two characters indicate the country of manufacture, and the last five digits are a sequential number assigned to each mainframe.

Additional Information

For Agilent N6700 MPS mainframes, you can query the model number, serial number, firmware revision, backup and active firmware.

For power modules, you can query the model number, serial number, installed options, voltage, current and power rating.

Front Panel:	SCPI Command:
Select System\About\Frame . or Select System\About\Module .	For mainframe information: *IDN? For information about the power module in channel 1: SYST:CHAN:MOD? (@1) SYST:CHAN:OPT? (@1) SYST:CHAN:SER? (@1)

Firmware Upgrade

You can query the instrument's firmware revision either from the front panel or over the remote interface as previously described under "Additional Information".

To upgrade your instrument with the latest firmware revision, go to <http://www.agilent.com/find/N6700firmware>. The upgrade procedure consists of the following three steps:

- Download and install the Agilent N6700 Firmware Update Utility from the Web.
- Download and unzip the Agilent N6700 Firmware Update file from the Web.
- Run the Agilent N6700 Firmware Update Utility and update the firmware on your instrument.


NOTE

On mainframes with firmware revisions prior to D.00.00, the following functions are not available:

- Support for the Agilent N678xA power modules.

On mainframes with firmware revisions prior to C.00.00, the following functions are not available:

- Support for the 300 W power modules.
- The power allocation function for power modules.
- The ability to reverse the polarity of the output and sense connectors.
- Compliance with LXI class C.

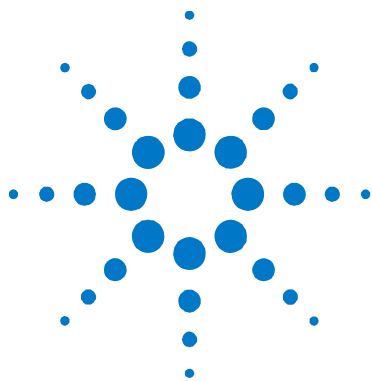

2

Performance Verification

Verification Description	9
Verification Procedure	13
Test Record Forms	13

The verification procedures described in this chapter verify that the Agilent N6700 Modular Power System is operating normally and is within published specifications.

NOTE

Perform the verification tests before calibrating your power system. If the power system passes the verification tests, the unit is operating within its calibration limits and does not need to be re-calibrated.

Verification procedures perform two primary functions:

Performance Tests These tests verify that the power system is operating normally and meets the specifications published in Appendix A in the User’s Guide.

Calibration Tests These tests verify that the power system is operating within its calibration limits.

If the instrument fails any of the tests or if abnormal test results are obtained, try calibrating the unit. If calibration is unsuccessful, return the unit to an Agilent Technologies Service Center.

Verification Description

Verification and Calibration Equipment Required

The equipment listed in the following table, or the equivalent to this equipment, is required for the performance tests and for calibration. Test record sheets are included at the back of this section.

Type	Specifications	Recommended Model
Digital Multimeter	Resolution: 10 nV @ 1V; Readout: 8 1/2 digits Accuracy: 20 ppm	Agilent 3458A or equivalent
Current Monitor	15 A (0.1 ohm), TC=4ppm/°C (all models exc. N6741B) 30 A (0.1 ohm), TC=4ppm/°C (model N6741B only)	Guilcline 9230A/15R Guilcline 9230A/30
Load Resistors	25 Ω , 250 W, 1%, TC<100 ppm/°C (calibration) 4 Ω , 250 W, 1%, TC<100 ppm/°C (calibration) 3.8 Ω , 250 W, 1%, TC<100 ppm/°C (N6754A calibration) 7.6 Ω , 250 W, 1%, TC<100 ppm/°C (N6754A calibration) 20 k Ω , 1%, 1/8W (verification, calibration for 1UA/2UA) 1 M Ω , 1%, 1/8W (calibration for N678xA only) 10 k Ω , 1%, 1/8W (calibration for N678xA only)	Vishay NH-250-25 Ω -1% Vishay NH-250-4 Ω -1%
Electronic Load	100 V, 20 A minimum, with transient capability and a slew rate of 833 kA/s or better.	Agilent N3300A mainframe, with N330xA modules
Agilent N6784A	Used as load for Agilent N678xA (set to CC load mode)	Agilent N6784A
GPIB Controller	Full GPIB capabilities	Agilent 82350B or equivalent
Oscilloscope	Sensitivity: 1 mV; Bandwidth Limit: 20 MHz Probe: 1:1 with RF tip	Agilent Infiniium or equivalent
RMS Voltmeter	True RMS; Bandwidth: 20 MHz Sensitivity: 100 μ V	Rhode and Schwartz Model URE3 or equivalent
Differential Amp.	Bandwidth: 20 MHz	LaCroy 1855A or equivalent
Terminations	1 – 50 Ω BNC termination 2 – 50 Ω , 1/8 W termination resistors	
Variable voltage transformer or AC source	Adjustable to highest rated input voltage range. Power: 500 VA	Agilent 6813B or equivalent
RC – for N678xA transient test	Capacitor: 150 μ F fixed film Resistor 50 m Ω	EPCOS B32526R0157K Vishay LVR01R0500FE70

Measurement Techniques

Voltmeter

To ensure that the values read by the voltmeter during both the verification procedure and the calibration procedure are not affected by the instantaneous measurement of the AC peaks of the output current ripple, make several DC measurements and average them.

If you are using an Agilent 3458A DMM, you can set up the voltmeter to do this automatically. From the instrument's front panel, program 100 power line cycles per measurement. Press NPLC 100 ENTER.

If you are using an Agilent 3458A DMM, turn on auto-calibration (ACAL) and the autorange function (ARANGE). For best results, auto-calibration should be performed every 24 hours when verifying or calibrating Agilent Models N678xA.

Current-Monitoring Resistor

The 4-terminal current shunt is used to eliminate output current measurement error caused by voltage drops in the load leads and connections. It has special current-monitoring terminals inside the load connection terminals. Connect the voltmeter directly to these current-monitoring terminals.

Electronic Load


Many of the test procedures require the use of a variable load capable of dissipating the required power. If a variable resistor is used, switches should be used to connect, disconnect, or short the load resistor. For most tests, an electronic load can be used. The electronic load is considerably easier to use than load resistors, but it may not be fast enough to test transient recovery time and may be too noisy for the noise (PARD) tests.

Fixed load resistors may be used in place of a variable load, with minor changes to the test procedures. Also, if computer controlled test setups are used, the relatively slow (compared to computers and system voltmeters) settling times and slew rates of the power system may have to be taken into account. "Wait" statements can be used in the test program if the test system is faster than the power system.

Unless stated otherwise, an Agilent Model N6784A power module should be used as the load when testing Agilent Models N678xA.

Verification Test Set-up

The following figures illustrate the test set-ups used for the verification procedures.

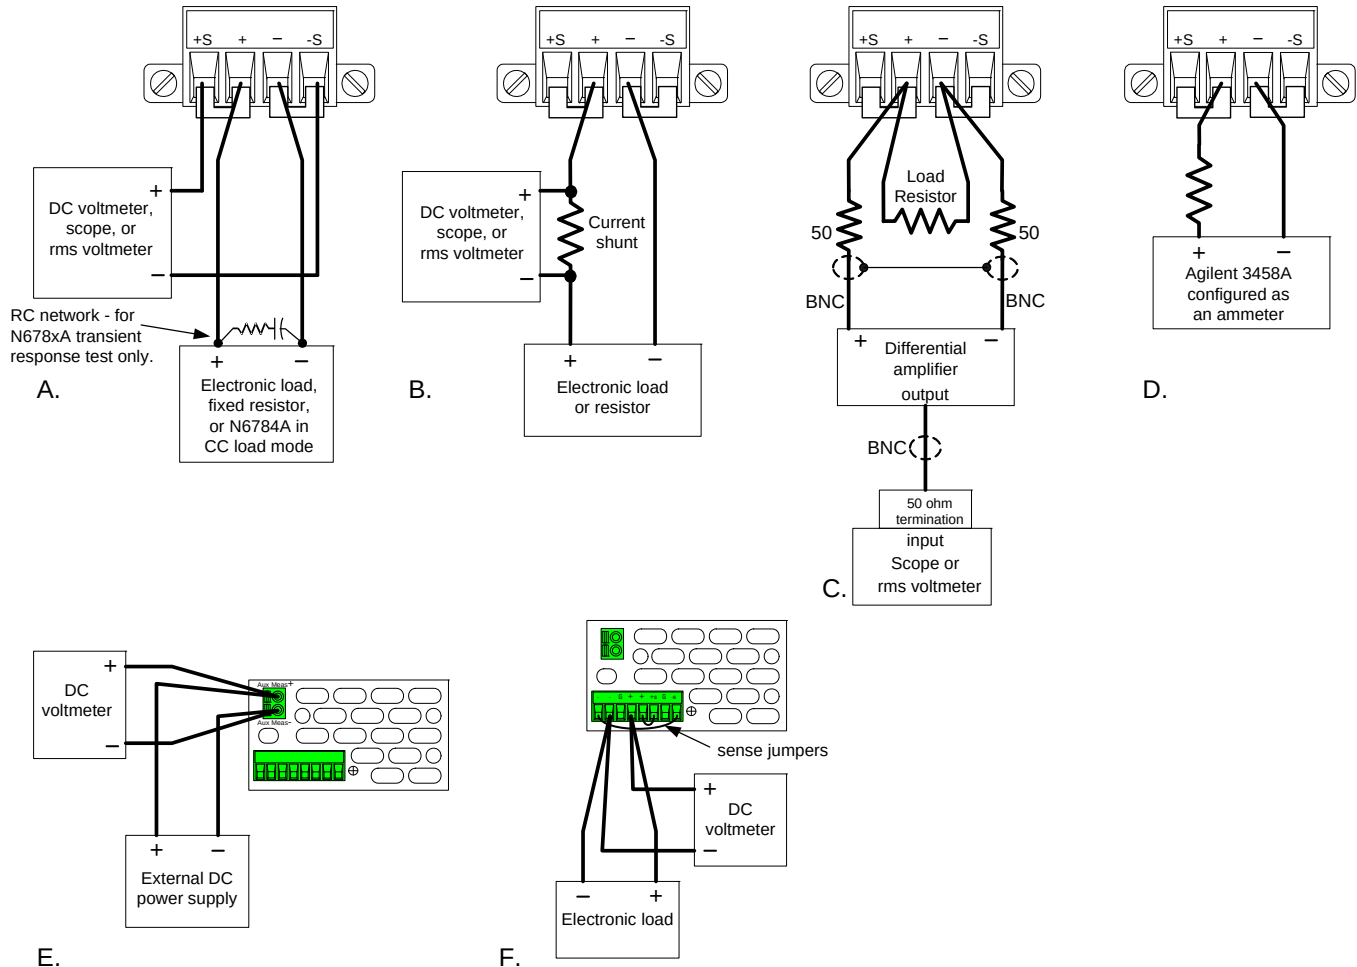

NOTE

Load lead lengths for Agilent Models N678xA must be between 1 and 4 feet.

Verification Procedure

Constant Voltage Tests

NOTE

Test each output channel individually. Refer to the appropriate test record form for the instrument settings of the model you are checking.

Voltage Programming and Readback Accuracy

Test category = performance, calibration

This test verifies that the voltage programming and measurement functions are within specifications.

- 1 Turn off the power system and connect a DMM across the sense terminals (see Test Setup A). Do **not** connect the load.
- 2 Turn on the power system and program the instrument settings as described in the test record form under “Voltage Programming & Readback, Min Voltage”. Turn the output on. The output status should be “CV” and the output current should be close to zero.
- 3 Record the output voltage reading from the DMM and the voltage measured over the interface. The readings should be within the limits specified in the test record form for the appropriate model under “Voltage Programming & Readback, Minimum Voltage”.
- 4 Program the instrument settings as described in the test record form under “Voltage Programming & Readback, High Voltage”.
- 5 Record the output voltage reading from the DMM and the voltage measured over the interface. The readings should be within the limits specified in the test record form for the appropriate model under “Voltage Programming & Readback, High Voltage”.
- 6 *For Agilent Models N676xA and N678xA only.* Set both the voltage programming and the voltage measurement to the low range (5.5 V for N676xA; 6 V programming and 1 V measurement for N678xA). Set the instrument as described under “Voltage Programming & Readback, Low Voltage”. Repeat step 5 for the low voltage range. The readings should be within the limits specified under “Low Range Voltage Programming & Readback”.
- 7 *For Agilent Models N678xA only.* Set the voltage programming to the 600 mV range and the voltage measurement to the 100 mV range. Set the instrument as described under “600 mV Programming & 100 mV Readback”. Repeat step 5. The readings should be within the limits specified under “600 mV Programming & 100 mV Readback”.

CV Load Effect

Test category = performance

This test measures the change in output voltage resulting from a change in output current from full load to no load.

- 1 Turn off the power system and connect a DMM and an electronic load (see Test Setup A).
- 2 Turn on the power system and program the instrument settings as described in the test record form under “CV Load Effect”.
- 3 Set the electronic load for the output channel’s current as described in the test record form under “CV Load Effect”. The output status should be “CV”. If it isn’t, adjust the load so that the output current drops slightly.
- 4 Record the output voltage reading from the DMM.
- 5 Open the load. Record the voltage reading from the DMM again. The difference between the DMM readings in steps 4 and 5 is the load effect, which should not exceed the value listed in the test record form for the appropriate model under “CV Load Effect”.
- 6 *For Agilent Models N678xA only.* Repeat steps 2 through 5 for the 6 V range.

CV Source Effect

Test category = performance

This test measures the change in output voltage that results from a change in AC line voltage from the minimum to maximum value within the line voltage specifications.

- 1 Turn off the power system and connect the ac power line through a variable voltage transformer or an AC source.
- 2 Connect a DMM and an electronic load (see Test Setup A). Set the transformer or AC source to nominal line voltage.
- 3 Turn on the power system and program the instrument settings as described in the test record form under “CV Source Effect”.
- 4 Set the electronic load for the output channel’s current as described in the test record form under “CV Source Effect”. The output status should be “CV”. If it isn’t, adjust the load so that the output current drops slightly.
- 5 Adjust the AC input to the lowest rated line voltage (86 VAC).
- 6 Record the output voltage reading from the DMM.
- 7 Adjust the AC input to the highest rated line voltage (264 VAC).
- 8 Record the output voltage reading on the DMM. The difference between the DMM reading in steps 6 and 8 is the source effect, which should not exceed the value listed in the test record form for the appropriate model under “CV Source Effect”.

CV Ripple and Noise

Test category = performance

Periodic and random deviations in the output combine to produce a residual AC voltage superimposed on the DC output voltage. This residual voltage is specified as the rms or peak-to-peak noise in the frequency range specified in Appendix A in the User's Guide.

- 1 Turn off the power system and connect a load resistor, differential amplifier, and an oscilloscope (ac coupled) to the output (see Test Setup C). For Agilent Models N678xA, observe the following additional connection requirements:
 - a. Twist the load leads, length must be between 1 and 4 ft.
 - b. Make all BNC connections directly at the load, not at the front panel terminals.
- 2 Use an appropriate load resistor to keep the power system at the instrument setting specified in the test record form under "CV Ripple and Noise".
- 3 As shown in the diagram, use two BNC cables to connect the differential amplifier to the + and – output terminals. Each cable should be terminated by a 50 Ω resistor. The shields of the two BNC cables should be connected together. Connect the output of the differential amplifier to the oscilloscope with a 50 Ω termination at the input of the oscilloscope.
- 4 Set the differential amplifier to multiply by ten, divide by one, and 1 M Ω input resistance. The positive and negative inputs of the differential amplifier should be set to AC coupling. Set the oscilloscope's time base to 5 ms/div, and the vertical scale to 10 mV/div. Turn the bandwidth limit on (usually 20 or 30 MHz), and set the sampling mode to peak detect.
- 5 Program the power system to the settings indicated in the in the test record form for the appropriate model under "CV Ripple and Noise" and enable the output. Let the oscilloscope run for a few seconds to generate enough measurement points. On the Agilent Infiniium scope, the maximum peak-to-peak voltage measurement is indicated at the bottom of the screen on the right side. Divide this value by 10 to get the CV peak-to-peak noise measurement. The result should not exceed the peak-to-peak limits in the test record form for the appropriate model under "CV Ripple and Noise, peak-to-peak".

NOTE

If the measurement contains any question marks, clear the measurement and try again. This means that some of the scope data received was questionable.


- 6 Disconnect the oscilloscope and connect an rms voltmeter in its place. Do not disconnect the 50 ohm termination. Divide the reading of the rms voltmeter by 10. The result should not exceed the rms limits in the test record form for the appropriate model under "CV Ripple and Noise, rms".
- 7 *For Agilent Models N678xA only.* Repeat steps 2 through 6 for the 6 V range.

Transient Recovery Time (all except Models N678xA)

Test category = performance

This test measures the time for the output voltage to recover to within the specified value following a 50% change in the load current.

- 1 Turn off the power system and connect an oscilloscope across the sense terminals (see Test Setup A). Connect an electronic load to the output terminals.
- 2 Turn on the power system and program the program the instrument settings as described in the test record form under “Transient Response”.
- 3 Set the electronic load to operate in constant current mode. Program its load current to the lower current value indicated in the test record form under “Transient Response”.
- 4 Set the electronic load's transient generator frequency to 100 Hz and its duty cycle to 50%.
- 5 Program the load's transient current level to the higher current value indicated in the test record form under “Transient Response”, and turn the transient generator on.
- 6 Adjust the oscilloscope for a waveform similar to that shown in the following figure.

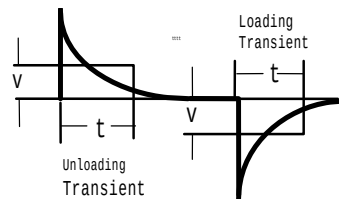

- 7 The output voltage should return to within the specified voltage at the specified time following the 50% load change. Check both loading and unloading transients by triggering on the positive and negative slope. Record the voltage at time “t” in the performance test record form under “Transient Response”.


Transient Recovery Time (Models N678xA only)

Test category = performance

This test measures the time for the output voltage to recover to within the specified value following a 50% change in the load currents of the 6 V range and the 20 V range.

- 1 Turn off the power system and connect an oscilloscope across the sense terminals (see Test Setup A). Connect an Agilent N6784A as a load to the output terminals. Observe the following additional connection requirements:
 - a. Twist the load leads, length must be between 1 and 4 ft.
 - b. Connect a 150 μ F capacitor and 50 m Ω resistor directly across the load.

- 2 Turn on the power system and program the Model N678xA instrument settings as described in the test record form under "Transient Response; 6V".
- 3 Set the Model N6784A that is being used as the load as follows:
 - a. Emulation Mode = CC Load
 - b. + Voltage limit = 6.12 V
 - c. Arb Current pulse properties:
 $I_0 = 0.1 \text{ A}$; $I_1 = 1.5 \text{ A}$; $T_0 = 1 \text{ ms}$; $T_1 = 1 \text{ ms}$; $T_2 = 1 \text{ ms}$;
 - d. Continuous = ON
 - e. Press Arb run.
- 4 Adjust the oscilloscope for a waveform similar to that shown in the following figure.

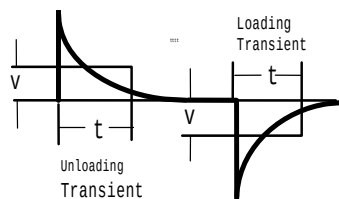

- 5 The output voltage should return to within the specified voltage at the specified time following the 50% load change. Check both loading and unloading transients by triggering on the positive and negative slope. Record the voltage at time "t" in the performance test record form under "Transient Response".
- 6 Repeat steps 3 through 5 for the 20 V range. Program the Model N678xA instrument settings as described on the test record form under "Transient Response; 20 V". Change the settings of the Model N6782A that is being used as the load as follows:
 - b. + Voltage limit = 20.4 V
 - c. Arb Current pulse properties:
 $I_0 = 0.1 \text{ A}$; $I_1 = 0.5 \text{ A}$;

Auxiliary Voltage Measurement Accuracy (N6781A only)

Test category = performance

This test verifies the auxiliary voltage measurement accuracy.

- 1 Turn off the power system and connect the external DMM and an external power supply to the auxiliary voltage inputs (see Test Setup E).
- 2 Turn on the external power supply and set the output to 20 volts. Turn on the power system. In Meter View, select Properties, and then select the Aux Voltage measurement input.
- 3 Record the external DMM reading and the auxiliary DVM readings. The auxiliary voltage reading should be within the designated voltage limit indicated in the test record form under "Auxiliary Voltage Readback".
- 4 Reverse the leads of the external power supply and repeat step 3.

Constant Current Tests

NOTE

Test each output channel individually. Refer to the appropriate test record form for the instrument settings of the model you are checking.

Current Programming and Readback Accuracy

Test category = performance, calibration

This test verifies that the current programming and measurement functions are within specifications.

- 1 Turn off the power system and connect the current shunt directly across the output terminals. Connect the DMM directly across the current shunt (see Test Setup B). Note that the electronic load is not used in this portion of the test.
- 2 Turn on the power system and program the instrument settings as described in the test record form under “Current Programming & Readback, Min Current”. The output status should be “CC”, and the output voltage should be close to zero.
- 3 Divide the voltage drop (DMM reading) across the current shunt by the shunt resistance to convert to amps and record this value (I_{out}). Also, record the current measured over the interface. The readings should be within the limits specified in the test record form for the appropriate model under “Current Programming & Readback, Minimum Current”.
- 4 Program the instrument settings as described in the test record form under “Current Programming & Readback, High Current”.
- 5 Divide the voltage drop (DMM reading) across the current shunt by the shunt resistance to convert to amps and record this value (I_{out}). Also, record the current reading measured over the interface. The readings should be within the limits specified in the test record form for the appropriate model under “Current Programming & Readback, High Current”.
- 6 *Step 6 for Agilent Models N676xA and N678xA only.* Set the current programming and current measurement to the low range - 100 mA for N676xA; 300 mA/100 mA programming and 100 mA measurement for N678xA. Set the instrument as described under “Current Programming & Readback, Low Current”. Repeat step 5. The readings should be within the limits specified under “Low Range Current Programming & Readback”.
- 7 *Steps 7 and 8 for Agilent Models N678xA only.* Set the current measurement to the 1 mA range. Set the instrument as described under “1 mA Range Readback”. Repeat step 5. The readings should be within the limits specified under “1 mA Range Readback”.

- 8 Set the current measurement to the 10 μA range. Set the instrument as described under “Current Readback, 10 μA ”. Repeat step 5. The readings should be within the limits specified under “10 μA Range Readback,”.
- 9 *Step 9 for Agilent Model N6784A only.* Set the current programming to the 10 mA range. Set the instrument as described under “10 mA Range Programming”. Divide the voltage drop (DMM reading) across the current shunt by the shunt resistance to convert to amps and record this value (I_{out}). The readings should be within the limits specified under “10 mA Range Programming”.
- 10 *Step 10 for Agilent Models N676xA with Option 2UA only.* Connect the Agilent 3458A and a 20k resistor to the output (see Test Setup D). Set the current measurement to the 200 μA range. Program the instrument settings as described in the test record form under “Current Readback, 200 μA Current”. Record the current reading of the 3458A and the current measured over the interface. Readings should be within limits specified for the appropriate model under “Current Readback, 200 μA Current”.

CC Load Effect

Test category = performance

This test measures the change in output current resulting from a change in output voltage from full scale to short circuit.

- 1 Turn off the power system and connect the current shunt, DMM, and electronic load (see Test Setup B). Connect the DMM directly across the current shunt.
- 2 Turn on the power system and program the instrument settings as described in the test record form under “CC Load Effect”.
- 3 Set the electronic load for CV mode and program it to the output channel’s voltage as described in the test record form under “CC Load Effect”. The output status should be “CC”. If it isn’t, adjust the load so that the output voltage drops slightly.
- 4 Divide the voltage drop (DMM reading) across the current monitoring resistor by its resistance to convert to amps and record this value (I_{out}).
- 5 Short the electronic load. Divide the voltage drop (DMM reading) across the current monitoring resistor by its resistance to convert to amps and record this value (I_{out}). The difference in the current readings in steps 4 and 5 is the load effect, which should not exceed the value listed in the test record form for the appropriate model under “CC Load Effect”.
- 6 *For Agilent Models N6781A and N6782A only.* Repeat steps 2 through 5 for the 1 A range and the 300 mA range.
- 7 *For Agilent Models N6784A only.* Repeat steps 2 through 5 for the 1 A range, the 100 mA range, and the 10 mA range.

CC Source Effect

Test category = performance

This test measures the change in output current that results from a change in AC line voltage from the minimum to maximum value within the line voltage specifications.

- 1 Turn off the power system and connect the ac power line through a variable voltage transformer or AC source.
- 2 Connect the current shunt, DMM, and electronic load (see Test Setup B). Connect the DMM directly across the current shunt. Set the transformer or AC source to nominal line voltage.
- 3 Turn on the power system and program the instrument settings as described in the test record form under “CC Source Effect”.
- 4 Set the electronic load for the output channel’s voltage under “CC Source Effect”. The output status should be “CC”. If it isn’t, adjust the load so that the output voltage drops slightly.
- 5 Adjust the AC input to the lowest rated line voltage (86 VAC).
- 6 Divide the voltage drop (DMM reading) across the current monitoring resistor by its resistance to convert to amps and record this value (I_{out}).
- 7 Adjust the AC input to the highest rated line voltage (264 VAC).
- 8 Divide the voltage drop (DMM reading) across the current monitoring resistor by its resistance to convert to amps and record this value (I_{out}). The difference between the DMM reading in steps 6 and 8 is the source effect, which should not exceed the value listed in the test record form for the appropriate model under “CC Source Effect”.

Resistance Programming Accuracy (N6781A only)

Test category = performance, calibration

Note: Current readback accuracy must be verified prior to this test.

- 1 Connect an external DMM and an electronic load directly to the output (see Test Setup F). Turn on the power system.
- 2 Set the 20 V range and program the output to 10 V. Turn the output on and record the voltage reading on the DMM. This is the voltage with no load (V_{nl}).
- 3 Program the output resistance to 1 ohm. Turn on the electronic load. Select CC mode, current: 1 A, voltage limit: 20 V, Input On.
- 4 Record the voltage reading on the DMM. This is the voltage with a load (V_{wl}). Record the current reading on the front panel of the power system. This is the current with a load (I_{wl}).
- 5 Calculate the resistance value as follows: $R = (V_{nl} - V_{wl}) / I_{wl}$
This is the output resistance, which should not exceed value listed in the test record from under “Resistance Programming”.
- 6 Repeat steps 2 through 5 for the 6 V range. Set the output voltage to 6 V and the load current to 3 A.

Test Record Forms

Test Record Form – Agilent N6731B and N6741B

Agilent N6731B and N6741B	Report No _____	Date _____
Description	Model	Minimum Specs. Results Maximum Specs.
Constant Voltage Tests		
Voltage Programming & Readback		
Minimum Voltage Vout	Both	– 4 mV _____ + 34 mV
Voltage measured over interface	Both	Vout – 20 mV _____ Vout + 20 mV
High Voltage Vout	Both	4.976 V _____ 5.024 V
Voltage measured over interface	Both	Vout – 25 mV _____ Vout + 25 mV
CV Load Effect	Both	– 5 mV _____ + 5 mV
CV Source Effect	Both	– 1 mV _____ + 1 mV
CV Ripple and Noise		
peak-to-peak	N6731B	N/A _____ + 10 mV
	N6741B	N/A _____ + 20 mV
rms	Both	N/A _____ + 2 mV
Transient Response		
Voltage at 200 μ s	N6731B	– 80 mV _____ + 80 mV
	N6741B	– 100 mV _____ + 100 mV
Constant Current Tests		
Current Programming & Readback		
Minimum Current Iout	Both	+ 40 mA _____ + 80 mA
Current measured over interface	Both	Iout – 20 mA _____ Iout + 20 mA
High Current Iout	N6731B	9.965 A _____ 10.035 A
	N6741B	19.95 A _____ 20.05 A
Current measured over interface	N6731B	Iout – 35 mA _____ Iout + 35 mA
	N6741B	Iout – 50 mA _____ Iout + 50 mA
CC Load Effect	Both	– 2 mA _____ + 2 mA
CC Source Effect	Both	– 1 mA _____ + 1 mA
Instrument Settings		
Test Description	N6731B	N6741B
Voltage Programming & Readback, Min Voltage	15 mV, 10 A	15 mV, 20 A
Voltage Programming & Readback, High Voltage	5 V, 10 A	5 V, 20 A
CV Load Effect, Source Effect, Ripple and Noise	5 V, 10 A	5 V, 20 A
Transient Response	5 V, from 5 A to 10 A	5 V, from 10 A to 20 A
Current Programming & Readback, Min Current	60 mA, 5 V	60 mA, 5 V
Current Programming & Readback, High Current	10 A, 5 V	20 A, 5 V
CC Load Effect, Source Effect	10 A, 5 V	20 A, 5 V

Test Record Form – Agilent N6732B and N6742B

Agilent N6732B and N6742B	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	– 4 mV		+ 34 mV
Voltage measured over interface	Both	Vout – 20 mV		Vout + 20 mV
High Voltage Vout	Both	7.973 V		8.027 V
Voltage measured over interface	Both	Vout – 28 mV		Vout + 28 mV
CV Load Effect				
	Both	– 6 mV		+ 6 mV
CV Source Effect				
	Both	– 2 mV		+ 2 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A		+ 12 mV
rms	Both	N/A		+ 2 mV
Transient Response				
Voltage at 200 μ s	N6732B	– 80 mV		+ 80 mV
	N6742B	– 100 mV		+ 100 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	– 20 mA		+ 60 mA
Current measured over interface	Both	Iout – 10 mA		Iout + 10 mA
High Current Iout	N6732B	6.2206 A		6.2794 A
	N6742B	12.46 A		12.54 A
Current measured over interface	N6732B	Iout – 19.37 mA		Iout + 19.37 mA
	N6742B	Iout – 29 mA		Iout + 29 mA
CC Load Effect				
	Both	– 2 mA		+ 2 mA
CC Source Effect				
	Both	– 1 mA		+ 1 mA
Instrument Settings				
Test Description	N6732B		N6742B	
Voltage Programming & Readback, Min Voltage	15 mV, 6.25 A		15 mV, 12.5 A	
Voltage Programming & Readback, High Voltage	8 V, 6.25 A		8 V, 12.5 A	
CV Load Effect, Source Effect, Ripple and Noise	8 V, 6.25 A		8 V, 12.5 A	
Transient Response	8 V, from 3.125 A to 6.25 A		8V, from 6.25A to 12.5A	
Current Programming & Readback, Min Current	40 mA, 8 V		40 mA, 8 V	
Current Programming & Readback, High Current	6.25 A, 8 V		12.5 A, 8 V	
CC Load Effect, Source Effect	6.25 A, 8 V		12.5 A, 8 V	

Test Record Form – Agilent N6733B and N6743B

Agilent N6733B and N6743B	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	+ 10 mV		+ 50 mV
Voltage measured over interface	Both	Vout – 20 mV		Vout + 20 mV
High Voltage Vout	Both	19.96 V		20.04 V
Voltage measured over interface	Both	Vout – 40 mV		Vout + 40 mV
CV Load Effect				
	Both	– 9 mV		+ 9 mV
CV Source Effect				
	Both	– 2 mV		+ 2 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A		+ 14 mV
rms	Both	N/A		+ 3 mV
Transient Response				
Voltage at 200 μ s	N6733B	– 200 mV		+ 200 mV
	N6743B	– 300 mV		+ 300 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	– 10 mA		+ 30 mA
Current measured over interface	Both	Iout – 5 mA		Iout + 5 mA
High Current Iout	N6733B	2.4762 A		2.5237 A
	N6743B	4.9725 A		5.0275 A
Current measured over interface	N6733B	Iout – 8.75 mA		Iout + 8.75 mA
	N6743B	Iout – 12.5 mA		Iout + 12.5 mA
CC Load Effect				
	Both	– 2 mA		+ 2 mA
CC Source Effect				
	Both	– 1 mA		+ 1 mA
Instrument Settings				
Test Description	N6733B	N6743B		
Voltage Programming & Readback, Min Voltage	30 mV, 2.5 A	30 mV, 5 A		
Voltage Programming & Readback, High Voltage	20 V, 2.5 A	20 V, 5 A		
CV Load Effect, Source Effect, Ripple and Noise	20 V, 2.5 A	20 V, 5 A		
Transient Response	20 V, from 1.25 A to 2.5 A	20 V, from 2.5 A to 5 A		
Current Programming & Readback, Min Current	10 mA, 20 V	10 mA, 20 V		
Current Programming & Readback, High Current	2.5 A, 20 V	5 A, 20 V		
CC Load Effect, Source Effect	2.5 A, 20 V	5 A, 20 V		

Test Record Form – Agilent N6734B and N6744B

Agilent N6734B and N6744B	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	+ 5 mV		+ 75 mV
Voltage measured over interface	Both	Vout – 35 mV		Vout + 35 mV
High Voltage Vout	Both	34.93 V		35.07 V
Voltage measured over interface	Both	Vout – 70 mV		Vout + 70 mV
CV Load Effect				
	Both	– 11 mV		+ 11 mV
CV Source Effect				
	Both	– 4 mV		+ 4 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A		+ 15 mV
rms	Both	N/A		+ 5 mV
Transient Response				
Voltage at 200 μ s	N6734B	– 200 mV		+ 200 mV
	N6744B	– 300 mV		+ 300 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	– 15 mA		+ 25 mA
Current measured over interface	Both	Iout – 4 mA		Iout + 4 mA
High Current Iout	N6734B	1.47775 A		1.52225 A
	N6744B	2.9755 A		3.0245 A
Current measured over interface	N6734B	Iout – 6.25 mA		Iout + 6.25 mA
	N6744B	Iout – 8.5 mA		Iout + 8.5 mA
CC Load Effect				
	Both	– 2 mA		+ 2 mA
CC Source Effect				
	Both	– 1 mA		+ 1 mA
Instrument Settings				
Test Description	N6734B		N6744B	
Voltage Programming & Readback, Min Voltage	40 mV, 1.5 A		40 mV, 3 A	
Voltage Programming & Readback, High Voltage	35 V, 1.5 A		35 V, 3 A	
CV Load Effect, Source Effect, Ripple and Noise	35 V, 1.5 A		35 V, 3 A	
Transient Response	35 V, from 0.75 A to 1.5 A		35 V, from 1.5 A to 3 A	
Current Programming & Readback, Min Current	5 mA, 35 V		5 mA, 35 V	
Current Programming & Readback, High Current	1.5 A, 35 V		3 A, 35 V	
CC Load Effect, Source Effect	1.5 A, 35 V		3 A, 35 V	

Test Record Form – Agilent N6735B and N6745B

Agilent N6735B and N6745B	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	+ 10 mV		+ 130 mV
Voltage measured over interface	Both	Vout – 60 mV		Vout + 60 mV
High Voltage Vout	Both	59.88 V		60.12 V
Voltage measured over interface	Both	Vout – 120 mV		Vout + 120 mV
CV Load Effect				
	N6735B	– 13 mV		+ 13 mV
	N6745B	– 16 mV		+ 16 mV
CV Source Effect				
	Both	– 6 mV		+ 6 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A		+ 25 mV
rms	Both	N/A		+ 9 mV
Transient Response				
Voltage at 200 μ s	N6735B	– 400 mV		+ 400 mV
	N6745B	– 500 mV		+ 500 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	– 17.5 mA		+ 22.5 mA
Current measured over interface	Both	Iout – 4 mA		Iout + 4 mA
High Current Iout	N6735B	0.7788 A		0.8212 A
	N6745B	1.5776 A		1.6224 A
Current measured over interface	N6735B	Iout – 5.2 mA		Iout + 5.2 mA
	N6745B	Iout – 6.4 mA		Iout + 6.4 mA
CC Load Effect				
	Both	– 2 mA		+ 2 mA
CC Source Effect				
	Both	– 1 mA		+ 1 mA
Instrument Settings				
Test Description	N6735B	N6745B		
Voltage Programming & Readback, Min Voltage	70 mV, 0.8 A	70 mV, 1.6 A		
Voltage Programming & Readback, High Voltage	60 V, 0.8 A	60 V, 1.6 A		
CV Load Effect, Source Effect, Ripple and Noise	60 V, 0.8 A	60 V, 1.6 A		
Transient Response	60 V, from 0.4 A to 0.8 A	60 V, from 0.8 A to 1.6 A		
Current Programming & Readback, Min Current	2.5 mA, 60 V	2.5 mA, 60 V		
Current Programming & Readback, High Current	0.8 A, 60 V	1.6 A, 60 V		
CC Load Effect, Source Effect	0.8 A, 60 V	1.6 A, 60 V		

Test Record Form – Agilent N6736B and N6746B

Agilent N6736B and N6746B	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	0 mV		+ 200 mV
Voltage measured over interface	Both	Vout – 100 mV		Vout + 100 mV
High Voltage Vout	Both	99.8 V		100.2 V
Voltage measured over interface	Both	Vout – 200 mV		Vout + 200 mV
CV Load Effect				
	N6736B	– 20 mV		+ 20 mV
	N6746B	– 30 mV		+ 30 mV
CV Source Effect				
	Both	– 10 mV		+ 10 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A		+ 30 mV
rms	Both	N/A		+ 18 mV
Transient Response				
Voltage at 200 μ s	N6736B	– 500 mV		+ 500 mV
	N6746B	– 1000 mV		+ 1000 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	– 8.5 mA		+ 11.5 mA
Current measured over interface	Both	Iout – 2 mA		Iout + 2 mA
High Current Iout	N6736B	0.4893 A		0.5107 A
	N6746B	0.9885 A		1.0115 A
Current measured over interface	N6736B	Iout – 2.75 mA		Iout + 2.75 mA
	N6746B	Iout – 3.5 mA		Iout + 3.5 mA
CC Load Effect				
	Both	– 2 mA		+ 2 mA
CC Source Effect				
	Both	– 1 mA		+ 1 mA
Instrument Settings				
Test Description	N6736B		N6746B	
Voltage Programming & Readback, Min Voltage	100 mV, 0.5 A		100 mV, 1 A	
Voltage Programming & Readback, High Voltage	100 V, 0.5 A		100 V, 1 A	
CV Load Effect, Source Effect, Ripple and Noise	100 V, 0.5 A		100 V, 1 A	
Transient Response	100 V, from 0.25 A to 0.5 A		100 V, from 0.5 A to 1 A	
Current Programming & Readback, Min Current	1.5 mA, 100 V		1.5 mA, 100 V	
Current Programming & Readback, High Current	0.5 A, 100 V		1 A, 100 V	
CC Load Effect, Source Effect	0.5 A, 100 V		1 A, 100 V	

Test Record Form – Agilent N6751A and N6752A

Agilent N6751A and N6752A	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	+ 1 mV		+ 39 mV
Voltage measured over interface	Both	Vout – 20 mV		Vout + 20 mV
High Voltage Vout	Both	49.951 V		50.049 V
Voltage measured over interface	Both	Vout – 45 mV		Vout + 45 mV
CV Load Effect				
	Both	– 2 mV		+ 2 mV
CV Source Effect				
	Both	– 1 mV		+ 1 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A		+ 4.5 mV
rms	Both	N/A		+ 0.35 mV
Transient Response				
Voltage at 100 μ s	Both	– 75 mV		+ 75 mV
Voltage at 100 μ s with Option 761	N6752A	– 125 mV		+ 125 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	– 10 mA		+ 30 mA
Current measured over interface	Both	Iout – 4 mA		Iout + 4 mA
High Current Iout	N6751A	4.975 A		5.025 A
	N6752A	9.970 A		10.030 A
Current measured over interface	N6751A	Iout – 9 mA		Iout + 9 mA
	N6752A	Iout – 14 mA		Iout + 14 mA
CC Load Effect				
	Both	– 2 mA		+ 2 mA
CC Source Effect				
	Both	– 1 mA		+ 1 mA

Instrument Settings		
Test Description	N6751A	N6752A
Voltage Programming & Readback, Min Voltage	20 mV, 5 A	20 mV, 10 A
Voltage Programming & Readback, High Voltage	50 V, 1 A	50 V, 2 A
CV Load Effect, Source Effect, Ripple and Noise	50 V, 1 A	50 V, 2 A
Transient Response	50 V, from 0.6 A to 1 A	50 V, from 1 A to 2 A
Current Programming & Readback, Min Current	10 mA, 50 V	10 mA, 50 V
Current Programming & Readback, High Current	5 A, 10 V	10 A, 8.5 V
CC Load Effect, Source Effect	5 A, 10 V	10 A, 8.5 V

Test Record Form – Agilent N6753A

Agilent N6753A	Report No _____	Date _____
Description	Model	Minimum Specs. Results Maximum Specs.
Constant Voltage Tests		
Voltage Programming & Readback		
Minimum Voltage Vout	0 mV	_____ + 20 mV
Voltage measured over interface	Vout – 10 mV	_____ Vout + 10 mV
High Voltage Vout	19.978 V	_____ 20.022 V
Voltage measured over interface	Vout – 20 mV	_____ Vout + 20 mV
CV Load Effect		
	– 2 mV	_____ + 2 mV
CV Source Effect		
	– 0.5 mV	_____ + 0.5 mV
CV Ripple and Noise		
peak-to-peak	N/A	_____ + 5 mV
rms	N/A	_____ + 1 mV
Transient Response		
Voltage at 100 μ s	– 30 mV	_____ + 30 mV
Voltage at 100 μ s w/Option 760/761	– 200 mV	_____ + 200 mV
Constant Current Tests		
Current Programming & Readback		
Minimum Current Iout	+ 20 mA	_____ + 80 mA
Current measured over interface	Iout – 30 mA	_____ Iout + 30 mA
High Current Iout	49.920 A	_____ 50.080 A
Current measured over interface	Iout – 80 mA	_____ Iout + 80 mA
CC Load Effect		
	– 12 mA	_____ + 12 mA
CC Source Effect		
	– 5 mA	_____ + 5 mA
N6753A Setting		
Test Description	N6753A Setting	
Voltage Programming & Readback, Min Voltage	10 mV, 50 A	
Voltage Programming & Readback, High Voltage	20 V, 50 A	
CV Load Effect, Source Effect, Ripple and Noise	20 V, 50 A	
Transient Response	20 V, from 25 A to 50 A	
Current Programming & Readback, Min Current	50 mA, 20 V	
Current Programming & Readback, High Current	50 A, 20 V	
CC Load Effect, Source Effect	50 A, 20 V	

Test Record Form – Agilent N6754A

Agilent N6754A	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout		0 mV		+ 50 mV
Voltage measured over interface		Vout – 25 mV		Vout + 25 mV
High Voltage Vout		59.939 V		60.061 V
Voltage measured over interface		Vout – 55 mV		Vout + 55 mV
CV Load Effect				
		– 2 mV		+ 2 mV
CV Source Effect				
		– 1 mV		+ 1 mV
CV Ripple and Noise				
peak-to-peak		N/A		+ 6 mV
rms		N/A		+ 1 mV
Transient Response				
Voltage at 100 μ s		– 90 mV		+ 90 mV
Voltage at 100 μ s w/Option 760/761		– 350 mV		+ 350 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout		+ 8 mA		+ 32 mA
Current measured over interface		Iout – 8 mA		Iout + 8 mA
High Current Iout		19.968 A		20.032 A
Current measured over interface		Iout – 28 mA		Iout + 28 mA
CC Load Effect				
		– 5 mA		+ 5 mA
CC Source Effect				
		– 2 mA		+ 2 mA
Test Description				
Test Description		N6754A Setting		
Voltage Programming & Readback, Min Voltage		25 mV, 20 A		
Voltage Programming & Readback, High Voltage		60 V, 20 A		
CV Load Effect, Source Effect, Ripple and Noise		60 V, 20 A		
Transient Response		60 V, from 10 A to 20 A		
Current Programming & Readback, Min Current		20 mA, 60 V		
Current Programming & Readback, High Current		20 A, 60 V		
CC Load Effect, Source Effect		20 A, 60 V		

Test Record Form – Agilent N6761A and N6762A

Agilent N6761A and N6762A Description	Report No _____ Model	Minimum Specs.	Date _____ Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	Both	+ 9 mV	_____	+ 21 mV
Voltage measured over interface	Both	Vout – 6 mV	_____	Vout + 6 mV
High Voltage Vout	Both	49.986 V	_____	50.014 V
Voltage measured over interface	Both	Vout – 14 mV	_____	Vout + 14 mV
Low Range Voltage Prog. & Readback				
Low Voltage Vout	Both	5.4976 V	_____	5.5024 V
Voltage measured over interface	Both	Vout – 2.4 mV	_____	Vout + 2.4 mV
CV Load Effect	Both	– 0.5 mV	_____	+ 0.5 mV
CV Source Effect	Both	– 0.5 mV	_____	+ 0.5 mV
CV Ripple and Noise				
peak-to-peak	Both	N/A	_____	+ 4.5 mV
rms	Both	N/A	_____	+ 0.35 mV
Transient Response				
Voltage at 150 μ s	Both	– 75 mV	_____	+ 75 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	Both	+ 0.8 mA	_____	+ 1.2 mA
Current measured over interface	Both	Iout – 160 μ A	_____	Iout + 160 μ A
High Current Iout	N6761A	1.4992 A	_____	1.5008 A
	N6762A	2.9986 A	_____	3.0014 A
Current measured over interface	N6761A	Iout – 0.76 mA	_____	Iout + 0.76 mA
	N6762A	Iout – 1.36 mA	_____	Iout + 1.36 mA
Low Range Current Prog. & Readback				
Low Current (Full Scale) Iout	Both	0.099930 A	_____	0.100070 A
Current measured over interface	Both	Iout – 45 μ A	_____	Iout + 45 μ A
Current Readback				
100 μ A current measured over interface	Both	Iout – 0.6 μ A	_____	Iout + 0.6 μ A
200 μ A current measured over interface	Both	Iout – 1.1 μ A	_____	Iout + 1.1 μ A
CC Load Effect	Both	– 65 μ A	_____	+ 65 μ A
CC Source Effect	Both	– 30 μ A	_____	+ 30 μ A

Test Description	N6761A Settings	N6762A Settings
Voltage Programming & Readback, Min Voltage	15 mV, 1.5 A	15 mV, 3 A
Voltage Programming & Readback, High Voltage	50 V, 1 A	50 V, 2 A
Voltage Programming & Readback, Low Voltage	5.5 V, 1.5 A	5.5 V, 3 A
CV Load Effect, Source Effect, Ripple and Noise	50 V, 1 A	50 V, 2 A
Transient Response	50 V, from 0.6 A to 1 A	50 V, from 1 A to 2 A
Current Programming & Readback, Min Current	1 mA, 50 V	1 mA, 50 V
Current Programming & Readback, High Current	1.5 A, 33 V	3 A, 33 V
Current Programming & Readback, Low Current	0.1 A, 50 V	0.1 A, 50 V
Current Readback, 100 μ A Current	1 mA, 1.9 V	1 mA, 1.9 V
Current Readback, 200 μ A Current	1 mA, 3.9 V	1 mA, 3.9 V
CC Load Effect, Source Effect	1.5 A, 33 V	3 A, 33 V

Test Record Form – Agilent N6773A

Agilent Model N6773A	Report No _____	Date _____
Description	Model	Minimum Specs. Results Maximum Specs.
Constant Voltage Tests		
Voltage Programming & Readback		
Minimum Voltage Vout	+ 10 mV	_____ + 50 mV
Voltage measured over interface	Vout – 20 mV	_____ Vout + 20 mV
High Voltage Vout	19.96 V	_____ 20.04 V
Voltage measured over interface	Vout – 40 mV	_____ Vout + 40 mV
CV Load Effect		
	– 13 mV	_____ + 13 mV
CV Source Effect		
	– 2 mV	_____ + 2 mV
CV Ripple and Noise		
peak-to-peak	N/A	_____ + 20 mV
rms	N/A	_____ + 3 mV
Transient Response		
Voltage at 250 μ s	– 300 mV	_____ + 300 mV
Constant Current Tests		
Current Programming & Readback		
Minimum Current Iout	– 30 mA	_____ + 90 mA
Current measured over interface	Iout – 15 mA	_____ Iout + 15 mA
High Current Iout	14.9175 A	_____ 15.0825 A
Current measured over interface	Iout – 37.5 mA	_____ Iout + 37.5 mA
CC Load Effect		
	– 6 mA	_____ + 6 mA
CC Source Effect		
	– 1 mA	_____ + 1 mA
Test Settings		
Test Description	N6773A Setting	
Voltage Programming & Readback, Min	30 mV, 15 A	
Voltage Programming & Readback, High	20 V, 15 A	
CV Load Effect, Source Effect, Ripple and Noise	20 V, 15 A	
Transient Response	20 V, from 7.5 A to 15 A	
Current Programming & Readback, Min	30 mA, 20 V	
Current Programming & Readback, High	15 A, 20 V	
CC Load Effect, Source Effect	15 A, 20 V	

Test Record Form – Agilent N6774A

Agilent Model N6774A	Report No _____	Date _____
Description	Model	Minimum Specs. Results Maximum Specs.
Constant Voltage Tests		
Voltage Programming & Readback		
Minimum Voltage Vout	+ 5 mV	_____ + 75 mV
Voltage measured over interface	Vout – 35 mV	_____ Vout + 35 mV
High Voltage Vout	34.93 V	_____ 35.07 V
Voltage measured over interface	Vout – 70 mV	_____ Vout + 70 mV
CV Load Effect		
	– 16 mV	_____ + 16 mV
CV Source Effect		
	– 4 mV	_____ + 4 mV
CV Ripple and Noise		
peak-to-peak	N/A	_____ + 22 mV
rms	N/A	_____ + 5 mV
Transient Response		
Voltage at 250 μ s	– 300 mV	_____ + 300 mV
Constant Current Tests		
Current Programming & Readback		
Minimum Current Iout	– 45 mA	_____ + 75 mA
Current measured over interface	Iout – 12 mA	_____ Iout + 12 mA
High Current Iout	8.42725 A	_____ 8.57275 A
Current measured over interface	Iout – 24.75 mA	_____ Iout + 24.75 mA
CC Load Effect		
	– 6 mA	_____ + 6 mA
CC Source Effect		
	– 1 mA	_____ + 1 mA
N6774A Setting		
Test Description	N6774A Setting	
Voltage Programming & Readback, Min	40 mV, 8.5 A	
Voltage Programming & Readback, High	35 V, 8.5 A	
CV Load Effect, Source Effect, Ripple and Noise	35 V, 8.5 A	
Transient Response	35 V, from 4.25 A to 8.5 A	
Current Programming & Readback, Min	15 mA, 35 V	
Current Programming & Readback, High	8.5 A, 35 V	
CC Load Effect, Source Effect	8.5 A, 35 V	

Test Record Form – Agilent N6775A

Agilent Model N6775A	Report No _____	Date _____
Description	Model	Minimum Specs. Results Maximum Specs.
Constant Voltage Tests		
Voltage Programming & Readback		
Minimum Voltage Vout	+ 10 mV	_____ + 130 mV
Voltage measured over interface	Vout – 60 mV	_____ Vout + 60 mV
High Voltage Vout	59.88 V	_____ 60.12 V
Voltage measured over interface	Vout – 120 mV	_____ Vout + 120 mV
CV Load Effect		
	– 24 mV	_____ + 24 mV
CV Source Effect		
	– 6 mV	_____ + 6 mV
CV Ripple and Noise		
peak-to-peak	N/A	_____ + 35 mV
rms	N/A	_____ + 9 mV
Transient Response		
Voltage at 250 μ s	– 500 mV	_____ + 500 mV
Constant Current Tests		
Current Programming & Readback		
Minimum Current Iout	– 52.5 mA	_____ + 67.5 mA
Current measured over interface	Iout – 12 mA	_____ Iout + 12 mA
High Current Iout	4.9325 A	_____ 5.0675 A
Current measured over interface	Iout – 19.5 mA	_____ Iout + 19.5 mA
CC Load Effect		
	– 6 mA	_____ + 6 mA
CC Source Effect		
	– 1 mA	_____ + 1 mA
Test Description N6775A Setting		
Voltage Programming & Readback, Min	70 mV, 5 A	
Voltage Programming & Readback, High	60 V, 5 A	
CV Load Effect, Source Effect, Ripple and Noise	60 V, 5 A	
Transient Response	60 V, from 2.5 A to 5 A	
Current Programming & Readback, Min	7.5 mA, 60 V	
Current Programming & Readback, High	5 A, 60 V	
CC Load Effect, Source Effect	5 A, 60 V	

Test Record Form – Agilent N6776A

Agilent Model N6776A	Report No _____	Date _____
Description	Model	Minimum Specs. Results Maximum Specs.
Constant Voltage Tests		
Voltage Programming & Readback		
Minimum Voltage Vout	0 mV	_____ + 200 mV
Voltage measured over interface	Vout – 100 mV	_____ Vout + 100 mV
High Voltage Vout	99.8 V	_____ 100.2 V
Voltage measured over interface	Vout – 200 mV	_____ Vout + 200 mV
CV Load Effect		
	– 45 mV	_____ + 45 mV
CV Source Effect		
	– 10 mV	_____ + 10 mV
CV Ripple and Noise		
peak-to-peak	N/A	_____ + 45 mV
rms	N/A	_____ + 18 mV
Transient Response		
Voltage at 250 μ s	– 1000 mV	_____ + 1000 mV
Constant Current Tests		
Current Programming & Readback		
Minimum Current Iout	– 25.5 mA	_____ + 34.5 mA
Current measured over interface	Iout – 6 mA	_____ Iout + 6 mA
High Current Iout	2.9655 A	_____ 3.0345 A
Current measured over interface	Iout – 10.5 mA	_____ Iout + 10.5 mA
CC Load Effect		
	– 6 mA	_____ + 6 mA
CC Source Effect		
	– 1 mA	_____ + 1 mA
Test Description N6776A Setting		
Voltage Programming & Readback, Min	100 mV, 3 A	
Voltage Programming & Readback, High	100 V, 3 A	
CV Load Effect, Source Effect, Ripple and Noise	100 V, 3 A	
Transient Response	100 V, from 1.5 A to 3 A	
Current Programming & Readback, Min	4.5 mA, 100 V	
Current Programming & Readback, High	3 A, 100 V	
CC Load Effect, Source Effect	3 A, 100 V	


Test Record Form – Agilent N6781A, N6782A, and N6784A

Agilent N6781A, N6782A and N6784A	Report No	Date		
Description	Model	Minimum Specs.	Results	Maximum Specs.
Constant Voltage Tests				
Voltage Programming & Readback				
Minimum Voltage Vout	All	– 1.8 mV		+ 1.8 mV
Voltage measured over interface	All	Vout – 1.2 mV		Vout + 1.2 mV
High Voltage Vout	All	19.9932 V		20.0068 V
Voltage measured over interface	All	Vout – 6.2 mV		Vout + 6.2 mV
Low Range Voltage Prog. & Readback				
1 V Voltage Vout	All	0.999915 V		1.00085 V
Voltage measured over interface	All	Vout – 325 μ V		Vout + 325 μ V
600 mV Prog. & 100 mV Readback				
100 mV Voltage Vout	All	99.775 mV		100.225 mV
Voltage measured over interface	All	Vout – 75 μ V		Vout + 75 μ V
CV Load Effect				
20 V output range	All	– 700 μ V		+ 700 μ V
6 V output range	All	– 400 μ V		– 400 μ V
CV Source Effect				
	All	– 300 μ V		+ 300 μ V
CV Ripple and Noise				
peak-to-peak 20 V output range	All	N/A		+ 12 mV
rms 20 V output range	All	N/A		+ 1.2 mV
peak-to-peak 6 V output range	All	N/A		+ 12 mV
rms 6 V output range	All	N/A		+ 1.2 mV
Transient Response				
6 V output range at 35 μ s	All	– 20 mV		+ 20 mV
20 V output range at 35 μ s	All	– 10 mV		+ 10 mV
Auxiliary Voltage Readback	N6781A	Vout – 10 mV		Vout + 10 mV
Constant Current Tests				
Current Programming & Readback				
Minimum Current Iout	All	– 300 μ A		+ 300 μ A
Current measured over interface	All	Iout – 250 μ A		Iout + 250 μ A
High Current Iout	All	2.9985 A		3.0015 A
Current measured over interface	All	Iout – 1.15 mA		Iout + 1.15 mA
Low Range Current Prog. & Readback				
300 mA range Current Iout	N6781/82A	99.82 mA		100.18 mA
100 mA range Current Iout	N6784A	99.958 mA		100.042 mA
Current measured over interface	All	Iout – 35 μ A		Iout + 35 μ A
1 mA Range Readback				
Current measured over interface	All	Iout – 350 nA		Iout + 350 nA
10 μA Range Readback				
Current measured over interface	All	Iout – 10.5 nA		Iout + 10.5 nA
10 mA Range Programming				
10 mA Current Iout	N6784A	9.9925 mA		10.0075 mA

Constant Current Tests - continued				
CC Load Effect				
3 A output range	All	– 100 μ A	_____	+ 100 μ A
1 A output range	All	– 50 μ A	_____	+ 50 μ A
300 mA output range	N6781/82A	– 50 μ A	_____	+ 50 μ A
100 mA & 10 mA output ranges	N6784A	– 1 μ A	_____	+ 1 μ A
CC Source Effect	All	– 60 μ A	_____	+ 60 μ A
N6781A Resistance Tests				
Resistance Programming				
20 V output range	N6781A	0.995 Ω	_____	1.005 Ω
6 V output range	N6781A	0.9975 Ω	_____	1.0025 Ω

Instrument Settings – Agilent N678xA

Test Description	N6781A, N6782A, and N6784A Settings
Voltage Programming & Readback, Min Voltage	0 V, 1 A
Voltage Programming & Readback, High Voltage	20 V, 1 A
Voltage Programming & Readback, Low Voltage	1 V, 1 A
600 mV Programming & 100 mV Readback	0.1 V, 1 A
CV Load Effect, 20 V range	20 V, 1 A
CV Load Effect, 6 V range	6 V, 3 A
CV Load Effect, 600 mV range	100 mV, 3 A
CV Source Effect	20 V, 1 A
CV Ripple and Noise, 20 V range	20 V, 1 A
CV Ripple and Noise, 6 V range	6 V, 3 A
Transient Response, 6 V range	Voltage Priority; Comp.= HIGH3; 6V, from 0.1 to 1.5 A
Transient Response, 20 V range	Voltage Priority; Comp.= HIGH3; 20V, from 0.1 to 0.9 A
Current Programming & Readback, Min Current	0 A, 6 V
Current Programming & Readback, High Current	3 A, 6 V
Current Programming & Readback, Low Current	100 mA, 20 V
1 mA Range Readback	1 mA, 20 V
10 μ A Range Readback	10 μ A, 20 V
CC Load Effect, 3 A range	3 A, 6 V
CC Load Effect, 1 A range	1 A, 6 V
CC Load Effect, 300 mA range	100 mA, 6 V
CC Load Effect, 100 mA range	100 mA, 6 V
CC Load Effect, 10 mA range	10 mA, 6 V
CC Source Effect	3 A, 6 V
N6781A Resistance Programming, 20 V range	10 V, 1 Ω (load setting: CC mode, 20 V, 1A)
N6781A Resistance Programming, 6 V range	6 V, 1 Ω (load setting: CC mode, 20 V, 3A)

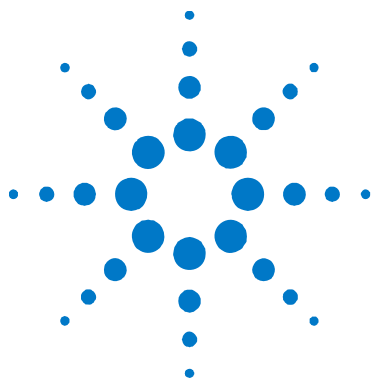

3 Calibration

Calibration Description	38
Calibration Procedure	39

This chapter includes calibration procedures for the Agilent N6700 Modular Power System. Instructions are given for performing the procedures from either the front panel or a controller over the GPIB.

Refer to the “Equipment Required” section in chapter 2 for a list of the equipment required for calibration. Also refer to “Measurement Techniques” for information about connecting the voltmeter and current shunt.

NOTE

Perform the verification tests before calibrating your power system. If the power system passes the verification tests, the unit is operating within its calibration limits and does not need to be re-calibrated.

Calibration Interval

The recommended calibration interval for Agilent N6700 Series power modules is one year. Agilent N6700A/B, N6701A, and N6702A MPS mainframes do not require calibration.

Calibration Description

Refer to the “Equipment Required” section in chapter 2 for a list of the equipment required for calibration. Also refer to “Measurement Techniques” for information about connecting the voltmeter and current shunt. Additional information about calibration follows:

- The correct password is required to enter the Admin menu, which contains the calibration function. The password is factory-set to 0 (zero). You can change the password once calibration mode is entered to prevent unauthorized access to the calibration mode. Refer to “Change the Calibration Password” at the end of this section.
- Calibrate only ONE channel at a time. The calibration commands accept only a single channel number for the channel parameter. Calibration cannot be performed on channels that have been grouped. If any channels have been grouped, they must be ungrouped before they can be calibrated.
- When calibrating the unit using SCPI commands, most steps involve sending a *OPC? query to synchronize with the power system’s command completion before proceeding. The response from the instrument must be read each time *OPC? is given. In some steps, it may take up to 30 seconds for *OPC? to respond.
- **Once started, you must perform the complete calibration procedure in its entirety.** As each calibration section is completed, the instrument calculates new calibration constants and begins using them. However, these constants are not saved in nonvolatile memory until a SAVE command is explicitly given.
- Exit the calibration mode either by logging out of the Admin menu or by sending CAL:STAT OFF. Note that any channels that were calibrated but not saved will revert to their previous calibration constants.


Calibration Switches

Two switches control the access to calibration commands. The switches are on the interface board and are accessible by removing the top cover. Refer to “Accessing the Calibration switch” in chapter 4. Switches 1 and 2 set the calibration configuration as follows:

	Sw 1	Sw 2	Description
Normal	ON	ON	This is the default or as-shipped switch setting. The calibration functions are accessible after entering a numeric password. The default password is 0 (zero).
Clear password	OFF	ON	The admin/calibration password is reset to 0 when the instrument is first powered on. Use this setting if you have forgotten the password.
Inhibit calibration	OFF	OFF	All calibration commands are disabled. This is useful where calibration access is guarded by instrument seals.

Calibration Set-up

The following figure shows the calibration test set-ups. Connect all leads to the Output terminals as shown in the following figure:

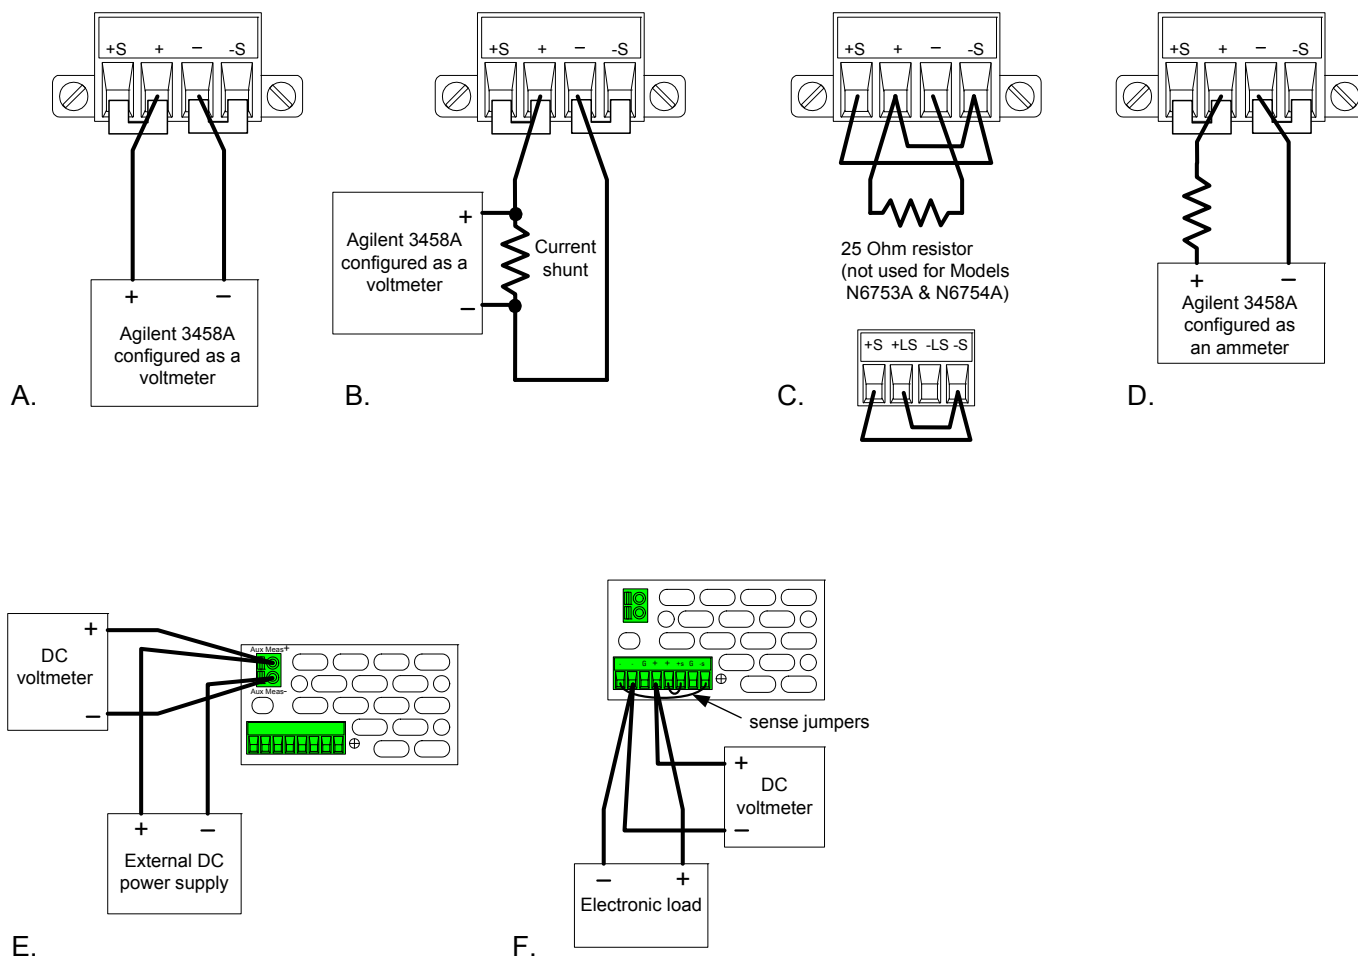

NOTE

Load lead lengths for Agilent Models N678xA must be between 1 and 4 feet.

Calibration Procedure – Models N673xB, N674xB, N677xA

Enter Calibration mode

Front Panel:	SCPI Command:
Select System\Admin>Login . Enter your password in the Password field and press Select.	CAL:STAT ON, <password>

Voltage Calibration

High Range Programming and Measurement

Step 1. Connect the voltage input of the Agilent 3458A DMM to an output channel (see Cal Setup A).

Step 2. Select the full-scale voltage programming and measurement range. The value entered must be the maximum voltage of the range that you are calibrating. The following example selects the 60 V full-scale range of output 1. Full-scale ranges vary according to model.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vprog . Then select the High range.	CAL:VOLT 60, (@1)

Step 3. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data	CAL:LEV P1 *OPC?

Step 4. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 5. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data	CAL:LEV P2 *OPC?

Step 6. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Current Calibration

High Range Programming and Measurement

The output voltage may go negative at some point during this procedure on units that have polarity reversal relays (Option 760).

Step 1. Connect a precision shunt resistor to the output. The shunt resistor should be able to measure at least 120% of the output's full-scale current (see Cal setup B). Connect the Agilent 3458A DMM across the shunt resistor.

Step 2. Select the full-scale current programming range. The value to program a range must be the maximum current of the range. The following example selects the 5 A full-scale range of output 1. Full-scale ranges vary according to model.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Iprog Then select the High range.	CAL:CURRE 5, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data	CAL:LEV P1 *OPC?

Step 4. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data	CAL:LEV P2 *OPC?

Step 6. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Downprogrammer Calibration

Step 1. Remove all loads from the output. This procedure is automatic and takes a few seconds.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\Dprog . Then select Next.	CAL:DPRog (@1) *OPC?

Enter a Calibration Date

Front Panel:	SCPI Command:
Select System\Admin\Cal\Date . Enter the calibration date in the Date field. If desired, you can enter alphanumeric data in this field.	To enter a calibration date: CAL:DATE "<date>", (@1)

Save and Log out of Calibration Mode

CAUTION

Storing calibration constants overwrites the existing ones in non-volatile memory. If you are not sure you want to permanently store the new constants, do not Save the data when you exit the calibration mode. The calibration will then remain unchanged.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Save . Select Save to save all calibration data.	To save calibration data: CAL:SAVE
Select System\Admin\Logout to exit calibration mode.	To exit calibration mode: CAL:STAT OFF

Calibration Procedure – Models N675xA

Enter Calibration mode

Front Panel:	SCPI Command:
Select System\Admin>Login . Enter your password in the Password field and press Select.	CAL:STAT ON, <password>

Voltage Calibration

High Range Programming and Measurement

- Step 1.** Connect the voltage input of the Agilent 3458A DMM to an output channel (see Cal Setup A).
- Step 2.** Select the full-scale voltage programming and measurement range. The value entered must be the maximum voltage of the range that you are calibrating. The following example selects the 60 V full-scale range of output 1. Full-scale ranges vary according to model.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vprog . Then select the High range.	CAL:VOLT 60, (@1)

- Step 3.** Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data	CAL:LEV P1 *OPC?

- Step 4.** Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

- Step 5.** Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data	CAL:LEV P2 *OPC?

Step 6. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Voltage Common Mode Rejection Ratio Calibration

Step 1. For this step, make the connections shown in Cal Setup C.

Connect an external jumper between the +sense and the –sense terminals. Connect a second jumper from the +output to the –sense terminal. Connect a 25 Ω load resistor across the +output and –output terminals. This resistor is **only** needed for Models N6751A and N6752A.

This procedure is automatic and only takes a few seconds.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\CMRR . Then select Next.	CAL:VOLT:CMRR (@1) *OPC?

After calibration completes, disconnect all jumpers and resistors.

Current Calibration

High Range Programming and Measurement

The output voltage may go negative at some point during this procedure on units that have polarity reversal relays (Option 760).

Step 1. Connect a precision shunt resistor to the output. The shunt resistor should be able to measure at least 120% of the output's full-scale current (see Cal Setup B). Connect the Agilent 3458A across the shunt resistor.

Step 2. Select the full-scale current programming range. The value to program a range must be the maximum current of the range. This example selects the 5 A full-scale range of output 1. Full-scale ranges vary according to model.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Iprog Then select the High range.	CAL:CURRE 5, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Peak Current Limit Calibration

Note for Models N6753A and N6754A, the peak current limit calibration is valid for 5 years.

Step 1. Connect only the appropriate resistor (see chapter 2) or electronic load across the output terminals for the first calibration point:

Model	1 st calibration point	2 nd calibration point
N6751A /N6752A:	25 Ω resistor	4 Ω resistor
N6753A:	0.6 Ω resistor (includes lead resistance) Electronic load set to 26.25A, CC mode	1.2 Ω resistor (includes lead resistance) Electronic load set to 13.12A, CC mode
N6754A:	3.8 Ω resistor (includes lead resistance) Electronic load set to 10.5A, CC mode	7.6 Ω resistor (includes lead resistance) Electronic load set to 5.25A, CC mode

Step 2. Select peak current limit calibration.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\lpeak .	CAL : CURR : PEAK (@1)

Step 3 Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The calibration is automatic.	CAL : LEV P1 *OPC?

Step 4. Connect the appropriate resistor or set the electronic load for the second calibration point.

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The calibration is automatic.	CAL : LEV P2 *OPC?

Downprogrammer Calibration - Agilent Models N6751A and N6752A only

Step 1. Remove all loads from the output. This procedure is automatic and takes a few seconds.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\Dprog . Then select Next.	CAL : DPRog (@1) *OPC?

Enter a Calibration Date

Front Panel:	SCPI Command:
Select System\Admin\Cal\Date . Enter the calibration date in the Date field. If desired, you can enter alphanumeric data in this field.	To enter a calibration date: CAL : DATE "<date>", (@1)

Save and Log out of Calibration Mode

CAUTION

Storing calibration constants overwrites the existing ones in non-volatile memory. If you are not sure you want to permanently store the new constants, do not Save the data when you exit the calibration mode. The calibration will then remain unchanged.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Save . Select Save to save all calibration data.	To save calibration data: CAL : SAVE
Select System\Admin\Logout to exit calibration mode.	To exit calibration mode: CAL : STAT OFF

Calibration Procedure – Models N676xA

Warm-up Period for Agilent Models N6761A and N6762A

Agilent Models N6761A and N6762A require a 30-minute warm-up period in the reset (*RST) state before starting calibration.

Enter Calibration mode

Front Panel:	SCPI Command:
Select System\Admin>Login . Enter your password in the Password field and press Select.	CAL:STAT ON, <password>

Voltage Calibration

High Range Programming and Measurement

- Step 1.** Connect the voltage input of the Agilent 3458A DMM to an output channel (see Cal Setup A).
- Step 2.** Select the full-scale voltage programming and measurement range. The value entered must be the maximum voltage of the range that you are calibrating. The following example selects the 60 V full-scale range of output 1. Full-scale ranges vary according to model.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vprog . Then select the High range.	CAL:VOLT 60, (@1)

- Step 3.** Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data	CAL:LEV P1 *OPC?

- Step 4.** Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

- Step 5.** Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data	CAL:LEV P2 *OPC?

Step 6. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Low Range Voltage Programming

Step 1. Select the low-voltage programming range. The value entered must be the maximum voltage of the range to be calibrated. This example selects the 5 V range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vprog . Then select the Low1 range.	CAL:VOLT 5, (@1)

Step 2. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data	CAL:LEV P1 *OPC?

Step 3. Measure the output voltage with the DMM and enter the data. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 4. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL:LEV P2 *OPC?

Step 5. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration..	CAL:DATA <data>

Low Range Voltage Measurement

Step 1. Select the low-voltage measurement range. The value entered must be the maximum voltage of the range to be calibrated. This example selects the 5 V measurement range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vmeas . Then select the Low1 range.	CAL : VOLT : MEAS 5, (@1)

Step 2. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 3. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 4. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 5. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Voltage Common Mode Rejection Ratio Calibration

Step 1. For this step, make the connections shown in Cal Setup C.

Connect an external jumper between the +sense and the –sense terminals. Connect a second jumper from the +output to the –sense terminal. Connect a 25 Ω load resistor across the +output and –output terminals. This resistor is **only** needed for Models N6751A and N6752A.

This procedure is automatic and only takes a few seconds.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\CMRR . Then select Next.	CAL : VOLT : CMRR (@1) *OPC?

After calibration completes, disconnect all jumpers and resistors.

Current Calibration

High Range Programming and Measurement

The output voltage may go negative at some point during this procedure on units that have polarity reversal relays (Option 760).

Step 1. Connect a precision shunt resistor to the output. The shunt resistor should be able to measure at least 120% of the output's full-scale current (see Cal Setup B). Connect the Agilent 3458A across the shunt resistor.

Step 2. Select the full-scale current programming range. The value to program a range must be the maximum current of the range. This example selects the 3 A full-scale range of output 1. Full-scale ranges vary according to model.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Iprog Then select the High range.	CAL : CURR 3, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration	CAL : DATA <data>

Low Range Current Programming

Step 1. Connect only the current measurement terminals of the Agilent 3458A to the output terminals.

Step 2. Select the low-current programming range. The value to program a range must be the maximum current of the range. This example selects the 0.1 A range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Iprog . Then select the Low1 range.	CAL : CURR 0.1, (@1)

Step 3. Select the first current calibration point. Wait a minimum of 5 minutes for the output current to stabilize.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point. Wait a minimum of 30 seconds for the output current to stabilize.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Low Range Current Measurement

Step 1. Connect only the current measurement terminals of the Agilent 3458A to the output terminals.

Step 2. Select the low current measurement range. The value to program a range must be the maximum current of the range. This example selects the 0.1 A range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\lmeas Then select the Low1 range.	CAL : CURR : MEAS 0.1, (@1)

Step 3. Select the first current calibration point. Then wait a minimum of 5 minutes for the internal temperature to stabilize.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data	CAL : LEV P1 *OPC?

Step 4. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Step 5. Disconnect the Agilent 3458A from the output terminals. Then select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Wait a minimum of 5 minutes for the internal temperature to stabilize. Then select the third current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data	CAL : LEV P3 *OPC?

100 μ A/200 μ A Range Measurement (for Option 1uA or 2uA only)

- Step 1.** Remove all loads from the output. Leave the sense terminals connected to the output terminals.
- Step 2.** Select either the 100 μ A current measurement range or the 200 μ A measurement range. Then wait 10 seconds.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\I meas Then select the Low2 range.	CAL:CURR:MEAS 0.0001, (@1) *OPC? or CAL:CURR:MEAS 0.0002, (@1) *OPC?

- Step 3.** Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The field indicates: Enter P1 data.	CAL:LEV P1

- Step 4.** Connect the Agilent 3458A and a 20 k Ω resistor to the output (see equipment list in chapter 2 and Cal Setup D).
- Step 5.** Measure the output current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data> *OPC?

Peak Current Limit

- Step 1.** Connect only a 25 Ω resistor (see chapter 2) across the output terminals for the first calibration point:
- Step 2.** Select peak current limit calibration.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\Ipeak .	CAL:CURR:PEAK (@1)

- Step 3** Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The calibration is automatic.	CAL:LEV P1 *OPC?

Step 4. Connect a 4 Ω resistor (see chapter 2) across the output terminals for the second calibration point.

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The calibration is automatic.	CAL : LEV P2 *OPC?

Downprogrammer Calibration

Step 1. Remove all loads from the output. This procedure is automatic and takes a few seconds.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\Dprog . Then select Next.	CAL : DPRog (@1) *OPC?

Enter a Calibration Date

Front Panel:	SCPI Command:
Select System\Admin\Cal\Date . Enter the calibration date in the Date field. If desired, you can enter alphanumeric data in this field.	To enter a calibration date: CAL : DATE "<date>", (@1)

Save and Log out of Calibration Mode

CAUTION

Storing calibration constants overwrites the existing ones in non-volatile memory. If you are not sure you want to permanently store the new constants, do not Save the data when you exit the calibration mode. The calibration will then remain unchanged.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Save . Select Save to save all calibration data.	To save calibration data: CAL : SAVE
Select System\Admin\Logout to exit calibration mode.	To exit calibration mode: CAL : STAT OFF

Calibration Procedure – Models N678xA

Enter Calibration mode

Front Panel:	SCPI Command:
Select System\Admin>Login . Enter your password in the Password field and press Select.	CAL:STAT ON, <password>

Voltage Calibration

High Range Programming and Measurement

Step 1. Connect the voltage input of the Agilent 3458A to an output channel (see Cal Setup A).

Step 2. Select the full-scale voltage programming and measurement range. The value entered must be the maximum voltage of the range that you are calibrating. This example selects the 20 V full-scale range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vprog . Then select the High range.	CAL:VOLT 20, (@1)

Step 3. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL:LEV P1 *OPC?

Step 4. Measure the output voltage with the DMM and enter the data. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 5. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL:LEV P2 *OPC?

Step 6. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Steps 7 and 8 only apply to Agilent Model N6784A.

Step 7. Select the third voltage calibration point for the negative range.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL:LEV P3 *OPC?

Step 8. Measure the output voltage with the DMM and enter the data. The value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Low Range Voltage Programming

Step 1. Select the low-voltage programming range. The value entered must be the maximum voltage of the range to be calibrated. This example selects the 6 V range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vprog . Then select the Low1 range.	CAL:VOLT 6, (@1)

Step 2. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL:LEV P1 *OPC?

Step 3. Measure the output voltage with the DMM and enter the data. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 4. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 5. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Step 6 only applies to Agilent Models N6781A and N6782A.

Step 6. Repeat steps 1 through 5 for the 600 mV range.

Steps 7 through 9 only apply to Agilent Model N6784A.

Step 7. Select the third voltage calibration point for the negative range.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL : LEV P3 *OPC?

Step 8. Measure the output voltage with the DMM and enter the data. The value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Step 9. Repeat steps 1 through 5, 7 and 8 for the 600 mV range.

Low Range Voltage Measurement

Step 1. Select the low-voltage measurement range. The value entered must be the maximum voltage of the range to be calibrated. This example selects the 1 V range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vmeas . Then select the Low1 range.	CAL : VOLT : MEAS 1, (@1)

Step 2. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 3. Measure the output voltage with the DMM and enter the data. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 4. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 5. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration	CAL : DATA <data>

Step 6 only applies to Agilent Models N6781A and N6782A.

Step 6. Repeat steps 1 through 5 for the 100 mV range.

Steps 7 through 9 only apply to Agilent Model N6784A.

Step 7. Select the third voltage calibration point for the negative range.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL : LEV P3 *OPC?

Step 8. Measure the output voltage with the DMM and enter the data. The value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Step 9. Repeat steps 1 through 5, 7 and 8 for the 100 mV range.

Positive Voltage Limit

Step 1. Select the positive voltage limit range. The value to program a range must be the maximum voltage of the range to be calibrated. This example selects the 20 V positive limit range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\Vlim	CAL : VOLT : LIM : POS 20, (@1)

Step 2. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 3. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 4. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 5. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Step 6. Repeat steps 1 through 5 for the 6 V positive limit range.

Auxiliary Voltage Measurement (Agilent Model N6781A only)

Step 1. Connect the auxiliary input terminals to the output terminals of Model N6781A. Also connect the voltage input of the Agilent 3458A to the output terminals of Model N6781A (see Cal Setup E).

Step 2. Select the auxiliary voltage measurement input.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Volt\lmeas Then select the Aux voltage range.	CAL : VOLT : MEAS : AUX (@1)

Step 3. Select the first voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Measure the output voltage with the DMM and enter the data. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second voltage calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 7. Select the third voltage calibration point for the negative range.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL : LEV P3 *OPC?

Step 8. Measure the output voltage with the DMM and enter the data. The value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration	CAL : DATA <data>

Current Calibration

High Range Programming and Measurement

Do not connect anything to the Sense terminals.

Step 1. Connect a precision shunt resistor to the output. The shunt resistor should be able to measure at least 120% of the output's rated full-scale current (see Cal Setup B). Connect the Agilent 3458A across the shunt resistor.

Step 2. Select the full-scale current programming range. The value to program a range must be the maximum current of the range. This example selects the 3 A full-scale range of output 1.

Note that this procedure calibrates both the 3 A and 1 A ranges.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Iprog Then select the High range.	CAL : CURR 3, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Calculate the shunt current ($I=V/R$) and enter the data. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point. Wait a minimum of 5 minutes for the internal temperature to stabilize.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 7. Select the third voltage calibration point for the negative range.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL : LEV P3 *OPC?

Step 8. Calculate the shunt current ($I=V/R$) and enter the data. The value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Low Range Current Programming

Step 1. Connect only the current measurement terminals of the Agilent 3458A to the output terminals.

Step 2. Select the low-current programming range. The value to program a range must be the maximum current of the range. This example selects the 300 mA range of output 1. All models have a 300 mA range. Model N6784A also has a 100 mA and a 10 mA range.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Iprog Then select the Low1 range.	CAL : CURR 0.3, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Measure the current with the Agilent 3458A and enter the value. This value may be positive or negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 7. Select the third current calibration point for the negative range.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL : LEV P3 *OPC?

Step 8. Measure the current with the Agilent 3458A and enter the value. This value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Step 9. Repeat steps 1 through 8 for the 100 mA programming range and again for the 10 mA programming range of Model N6784A.

100 mA Measurement Range

Step 1. Connect only the current measurement terminals of the Agilent 3458A to the output terminals.

Step 2. Select the 0.1 A range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Imeas Then select the Low1 range.	CAL : CURR : MEAS 0.1, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Measure the current with the Agilent 3458A and enter the value. This value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

1 mA Measurement Range

Step 1. Connect the Agilent 3458A in series with a 10 k Ω resistor to the output (see equipment list in chapter 2 and Cal Setup D).

Step 2. Select the 0.001 A range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Imeas Then select the Low2 range.	CAL : CURR : MEAS 0.001, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Measure the current with the Agilent 3458A and enter the value. This value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

10 μ A Measurement Range

Step 1. Connect the Agilent 3458A in series with a 1 M Ω resistor to the output (see equipment list in chapter 2 and Cal Setup D). Set the Agilent 3458A to measure current using the 100 μ A range (no autoranging). The remote command to do this is “DCI 100e-6”.

Step 2. Select the 10 μ A low-current measurement range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\I meas Then select the Low3 range.	CAL : CURR : MEAS 0.00001, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Measure the current with the Agilent 3458A and enter the value.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Measure the current with the Agilent 3458A and enter the value. This value should be negative.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Positive Current Limit

Step 1. Connect a precision shunt resistor to the output. The shunt resistor should be able to measure at least 120% of the output's rated full-scale current (see Cal Setup B). Connect the Agilent 3458A across the shunt resistor.

Step 2. Select the 3 A positive limit range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Curr\Lim.	CAL : CURR : LIM : POS 3, (@1)

Step 3. Select the first current calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL : LEV P1 *OPC?

Step 4. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL : DATA <data>

Step 5. Select the second voltage calibration point. Wait 5 minutes for the internal temperature to stabilize before continuing.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL : LEV P2 *OPC?

Step 6. Calculate the shunt current ($I=V/R$) and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL : DATA <data>

Resistance Calibration

Step 1. Connect an electronic load directly to the N6781A output (see Cal Setup F). Set the load to constant current mode, current to 0.95A. Also connect the Agilent 3458A to the N6781A output terminals.

Step 2. Select the 6 V resistance range of output 1.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Misc\Resistance . Then select the 6 V range.	CAL:RES 20 (@1) *OPC?

Step 3. Select the first resistance calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P1 data.	CAL:LEV P1 *OPC?

Step 4. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 5. Select the second resistance calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P2 data.	CAL:LEV P2 *OPC?

Step 6. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done.	CAL:DATA <data>

Step 7. Select the third resistance calibration point.

Front Panel:	SCPI Command:
Select Next. The information field should indicate: Enter P3 data.	CAL:LEV P2 *OPC?

Step 8. Measure the output voltage with the DMM and enter the data.

Front Panel:	SCPI Command:
Select the Measured Data field. Enter the data from the external DMM. Press Select when done. Press Next to finish calibration.	CAL:DATA <data>

Step 9. Repeat steps 1 through 8 for the 20 V resistance range of output 1.

Enter a Calibration Date

Front Panel:	SCPI Command:
Select System\Admin\Cal\Date . Enter the calibration date in the Date field. If desired, you can enter alphanumeric data in this field.	To enter a calibration date: CAL : DATE "<date>", (@1)

Save and Log out of Calibration Mode

CAUTION

Storing calibration constants overwrites the existing ones in non-volatile memory. If you are not sure you want to permanently store the new constants, do not Save the data when you exit the calibration mode. The calibration will then remain unchanged.

Front Panel:	SCPI Command:
Select System\Admin\Cal\Save . Select Save to save all calibration data.	To save calibration data: CAL : SAVE
Select System\Admin\Logout to exit calibration mode.	To exit calibration mode: CAL : STAT OFF

Change the Admin/Calibration Password


The password must be numeric, and can be up to 15 digits in length. After it has been changed, you can only enter the calibration mode by providing the correct password.

If the password is lost or forgotten, access can be restored by setting an internal switch that resets the password to zero (refer to “Accessing the Calibration switch” in chapter 4). Once you have set the password to zero with the switch, you can enter a new password using the Admin menu or using the CAL:PASS command. The new password will become active when you log out of the Admin Menu or send CAL STAT OFF. After you have returned the switches to the normal position, you can access the Admin menu with the new password.

Front Panel:	SCPI Command:
Select System\Admin>Login .	Enter calibration mode using the original password
Enter the original password in the Password field and press Select.	CAL:STAT ON, <password>
Select System\Admin>Password .	To change the password:
Enter a new password in the Password field.	CAL:PASS <Nrf>
Logout of the Admin menu to activate the password.	To exit calibration mode and activate the password:
	CAL:STAT OFF

NOTE

If the message “Locked out by internal switch setting” or “Calibration is inhibited by switch setting” appears, the internal switch is set to prevent the password from being changed (refer to “Accessing the Calibration switch” in chapter 4).

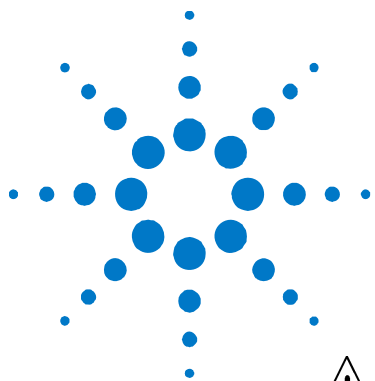

4 Disassembly

Electrostatic Discharge (ESD) Precautions	72
Disassembly Procedures	72
Installing a Redundant Ground for 400 Hz Operation	77

This chapter discusses the disassembly procedures for troubleshooting and repairing Agilent N6700B, N6701A, and N6702A MPS mainframes.

Electrostatic Discharge (ESD) Precautions

Almost all electrical components can be damaged by electrostatic discharge (ESD) during handling. Component damage can occur at electrostatic discharge voltages as low as 50 volts. The following guidelines will help prevent ESD damage when servicing the instrument or any electronic device.

- Disassemble instruments *only* in a static-free work area.
- Use a conductive work area to reduce static charges.
- Use a conductive wrist strap to reduce static accumulation.
- Minimize handling.
- Keep replacement parts in original static-free packaging.
- Remove all plastic, foam, vinyl, paper, and other static-generating materials from the immediate work area.



Disassembly Procedures

WARNING


SHOCK HAZARD. FAN HAZARD. Turn off the mainframe and disconnect its power cord before attempting any of the following procedures.

Required Disassembly Tools

Tool	Use
9/32 Hex driver	Removing GPIB connector
5/16 Hex driver	Removing DC cable assembly from bias supply
T20 Torx driver	Removing bias board, handles, and bulk supply
T10 Torx driver	Removing covers and board assemblies

Ribbon Cables

- Note the position of the conductive side of the cable for re-installation. (The blue tab is on the non-conductive side.)
- Release the ribbon cable by pulling up on the locking tab as shown by the arrows in the following figure.



- To replace the cable, fully insert the cable into the connector; then push down on the locking tab to secure the cable.


Removing/Installing Modules

CAUTION

Modules must be installed next to one another, starting with slot 1. Do not leave any empty slots *between* modules, otherwise the power system will not operate. Any remaining unused slots must have a filler module installed to ensure proper cooling. Do not install filler modules *between* power modules.

Step 1. Remove the blower cover. Remove three screws from the top of the cover and two screws on the sides. Tilt the cover up and slide it out.

Step 2. To remove a module, first remove the two fastening screws at either end of the module. Grasp the module at the ends (near the fan and the output connector), and lift it straight up out of the mainframe.

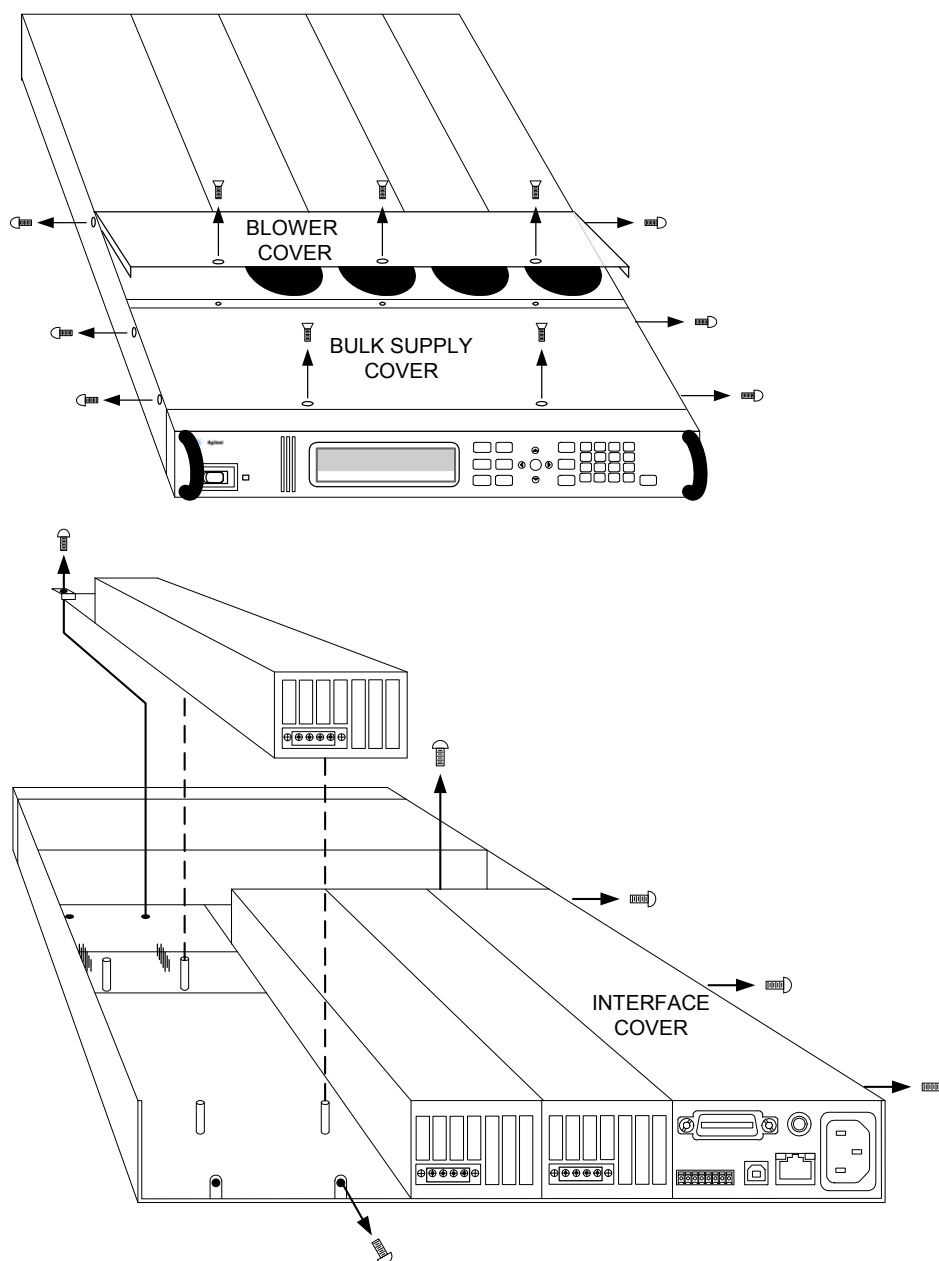

- Step 3.** To install a module, align the module over the alignment pins, and push it down onto the mainframe connector.
- Step 4.** Fasten the module to the mainframe. Install the two screws from the power module or filler module at either end of the module. Because the RFI strips are applying upward pressure, continue pushing down on the module until the screws are fully tightened.
- Step 5.** Replace the blower cover when finished.


Accessing the Calibration switch

- Step 1.** Remove the blower cover. Remove three screws from the top of the cover and two screws on the sides. Tilt the cover up and slide it out.
- Step 2.** Remove the interface cover. Remove the three screws along the left side of the unit. Then remove the screw at the front of the cover. Lift off the cover.
- Step 3.** The calibration switch is on the interface board near the ribbon cable. To change the calibration switch settings, use a small screwdriver to move the switches. Refer to chapter 3 for settings information.

CAUTION

Do not use a pencil to move the switches. Any graphite dust that gets on the switches will conduct electricity.

- Step 4.** Replace all covers when finished.

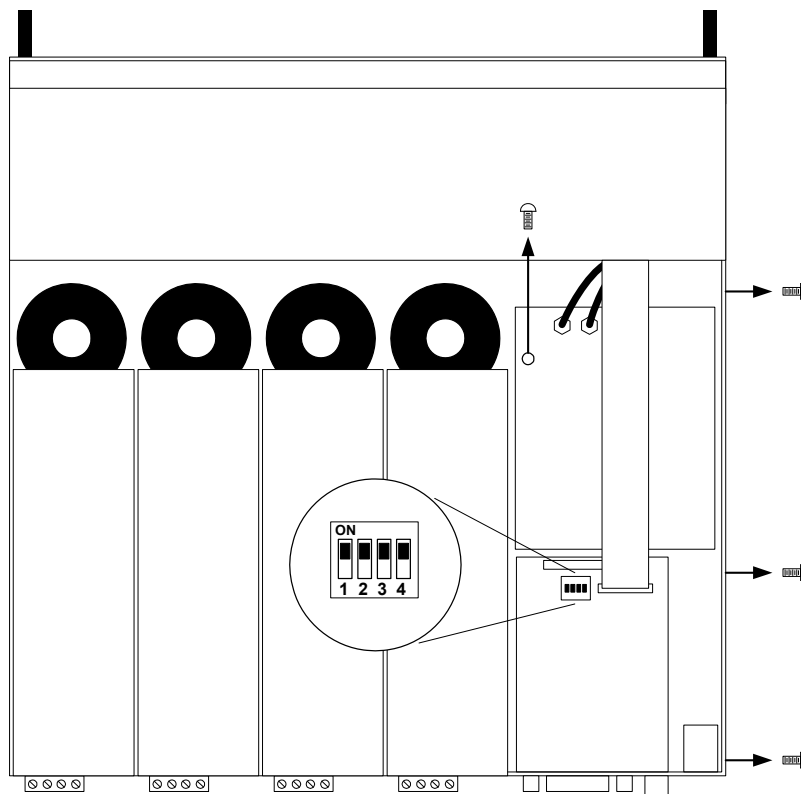

Removing/Installing the Interface (PPMC) board


- Step 1.** Remove the blower cover. Remove three screws from the top of the cover and two screws on the sides. Tilt the cover up and slide it out.
- Step 2.** Remove the interface cover. Remove the three screws along the left side of the unit. Then remove the screw at the front of the cover. Lift off the cover.
- Step 3.** Use a hex wrench to remove the GPIB connector from the rear of the mainframe. Disconnect all cable assemblies from the interface board.
- Step 4.** Disconnect the 3 cable assemblies located along the front edge of the board. Use a T10 driver and remove the screws that attach the board to the chassis. Lift the board out.
- Step 5.** To reinstall the interface board, perform the above steps in reverse order. Replace all covers when finished.

Removing/Installing the Bias board

- Step 1.** Remove the blower and interface covers as previously described.
- Step 2.** Disconnect all cable assemblies from the bias board.
- Step 3.** Use a T10 driver and remove the screws that attach the bias board to the chassis. Use a T20 driver and remove the 4 screws that attach the board to the backplane assembly. Lift the board out.
- Step 4.** To reinstall the bias board, perform the above steps in reverse order. Replace all covers when finished.

Removing/Installing the Front Panel Assembly

- Step 1.** Remove the two screws along the front of the bulk supply cover as well as the four screws on each side of the front panel assembly that attach the front panel assembly to the chassis.
- Step 2.** Slide the front panel assembly forward and away from the chassis to access the test points for troubleshooting.
- Step 3.** To completely remove the front panel assembly, disconnect the ribbon cable between the front panel board and the interface board at the front panel board.
- Step 4.** Disconnect the wires going to the S1 switch assembly. For reassembly, make a note of the color coding of the wires and the pins to which they are connected.

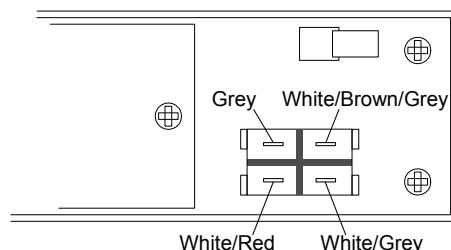

- Step 5.** To remove the front panel board, remove the six screws that secure the board to the front frame assembly.
- Step 6.** To remove the display module, first disconnect the cable at the P1 connector and the ribbon cable at the J2 connector. Then untwist the tabs that hold the display module to the front panel board.
- Step 7.** To reinstall the front panel assembly, perform the above steps in reverse order.

Removing/Installing the Bulk Supply

- Step 1.** Remove the blower cover, bulk supply cover, and interface cover as previously described.
- Step 2.** Remove the power module from slot #3 in the mainframe. You now have access to two of the screws that install the bulk supply.
- Step 3.** Remove the four screws on each side of the front panel assembly that attach the front panel assembly to the chassis. Slide the front panel assembly forward and away from the chassis. You now have access to the remaining screws that install the bulk supply.
- Step 4.** Use a T20 driver and remove all screws that fasten the bulk supply to the chassis.
- Step 5.** **For N6700B and N6701A mainframes**, slide the bulk supply over so that you can access the AC and DC cable assembly connectors.
For N6702A mainframes, which have two paralleled bulk supplies, disconnect the ribbon cable that connects the interface board to the front panel by gently lifting up on the interface board connector. Slide the ribbon cable out so that you can access the AC and DC cable assembly connectors.
- Step 6** Disconnect the DC and AC cable assemblies and lift the bulk supply out of the unit. For reassembly, make a note of the color-coding of the wires and the pins to which they are connected.

Cable assembly	Connected to Pin
Red (DC)	+48 V
Black (DC)	–48 V
Grey (AC)	AC
Red/white (AC)	ACC
Green/yellow (AC)	ground

- Step 7.** To reinstall the bulk supply, perform the above steps in reverse.

Installing a Redundant Ground for 400 Hz Operation

Operation at 400 Hz requires the installation of a redundant ground from the instrument chassis to earth ground. The redundant ground must be permanently attached to the unit as well as to the earth ground point.

The following procedure only describes how to make the permanent connection at the unit. The user must ensure the integrity and permanence of the connection at the earth ground point.


The following customer-supplied hardware is required:


- Ground wire (14/16 AWG)
- Uninsulated ring terminal for attaching wire to unit (Tyco p/n 34124 or equivalent)
- Hardware for attaching wire to earth ground point

The following tools are required for installing the redundant ground:

- 3/8 inch hex wrench

- Step 1.** Remove the top cover of the GPIB board as previously described under “Accessing the Calibration switch”.
- Step 2.** Use the wrench and remove the binding post (1) from the rear of the chassis. The binding post is located between the AC input connector and the GPIB connector.
- Step 3.** Crimp the appropriate ring terminal (2) onto the end of the ground wire.
- Step 4.** Place the ring terminal onto the threaded end of the binding post. Re-install the binding post on the chassis with the washer and nut (3).
- Step 5.** Rotate the ring terminal so that the ground wire does not interfere with any other connectors on the back of the unit. Use the wrench and tighten the binding post to the chassis (Torque = 20 – 25 in-lb.).

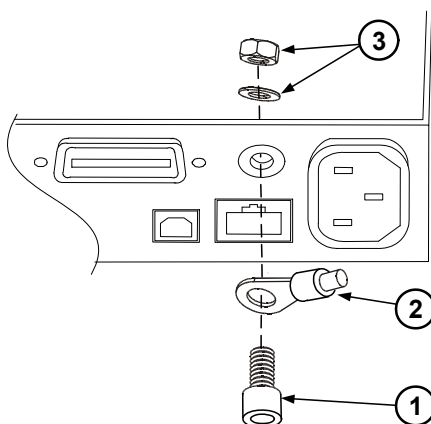

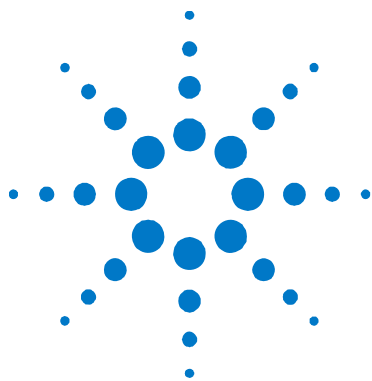

5 Troubleshooting

Preliminary Checkout	80
Overall Troubleshooting	81
Front Panel Troubleshooting	84
Bias Board Troubleshooting	84
Backplane Board Troubleshooting	85
Calibration and Passwords	86
Initialization	86

Before performing the Overall Troubleshooting procedures, perform the Preliminary Checkout procedure in the beginning of this chapter.

If the power system passes selftest and there are no obvious faults, perform the verification procedures in chapter 2 to determine if any power modules are not calibrated, or are not operating properly. This will help isolate a problem to a specific power module.

The following table documents the test equipment required for troubleshooting Agilent N6700 MPS mainframes.

Model	Description
Agilent 34401A or equivalent	Digital multimeter (for measuring voltage and resistance)

Preliminary Checkout

Is the instrument inoperative?

- Verify that the AC power cord is connected to the instrument.
- Verify that the front-panel On/Standby switch has been pushed.

Is the display working?

- If the display is hard to read, but front-panel LED is lit and the fans are working, the display contrast setting may be too light or too dark. Use the front panel menu to set the display contrast.

Does the instrument fail selftest?

- Remove all external connections to the instrument.
- Check that modules are installed next to each other, starting with slot 1. If there are any empty slots (or filler modules) *between* the power modules, the power system will not operate.
- Check that the mainframe has the latest firmware installed.
- Turn off the unit and cycle power to run selftest again.

If the supply passes selftest and there are no obvious faults, perform the verification procedures in chapter 2 to determine if any functions are not calibrated, or are not operating properly.

Self-test Error List

The following table documents the self-test error messages. Refer to Appendix A for other error messages.

Selftest Errors (these errors set Standard Event Status register bit #3)	
202	Selftest Fail Aux Adc 0 expected <n1> to <n2>, measured <n3>, chan <n4> Auxiliary ADC failed. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 0 expected <n1> to <n2>, measured <n3>, chan <n4> Both voltage and current DACs are at zero. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 1 expected <n1> to <n2>, measured <n3>, chan <n4> Voltage DAC is at zero; current DAC is at full scale. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 2 expected <n1> to <n2>, measured <n3>, chan <n4> Voltage DAC is at full scale; current DAC is at zero. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 3 expected <n1> to <n2>, measured <n3>, chan <n4> Both voltage and current DACs are at full scale. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.

Overall Troubleshooting

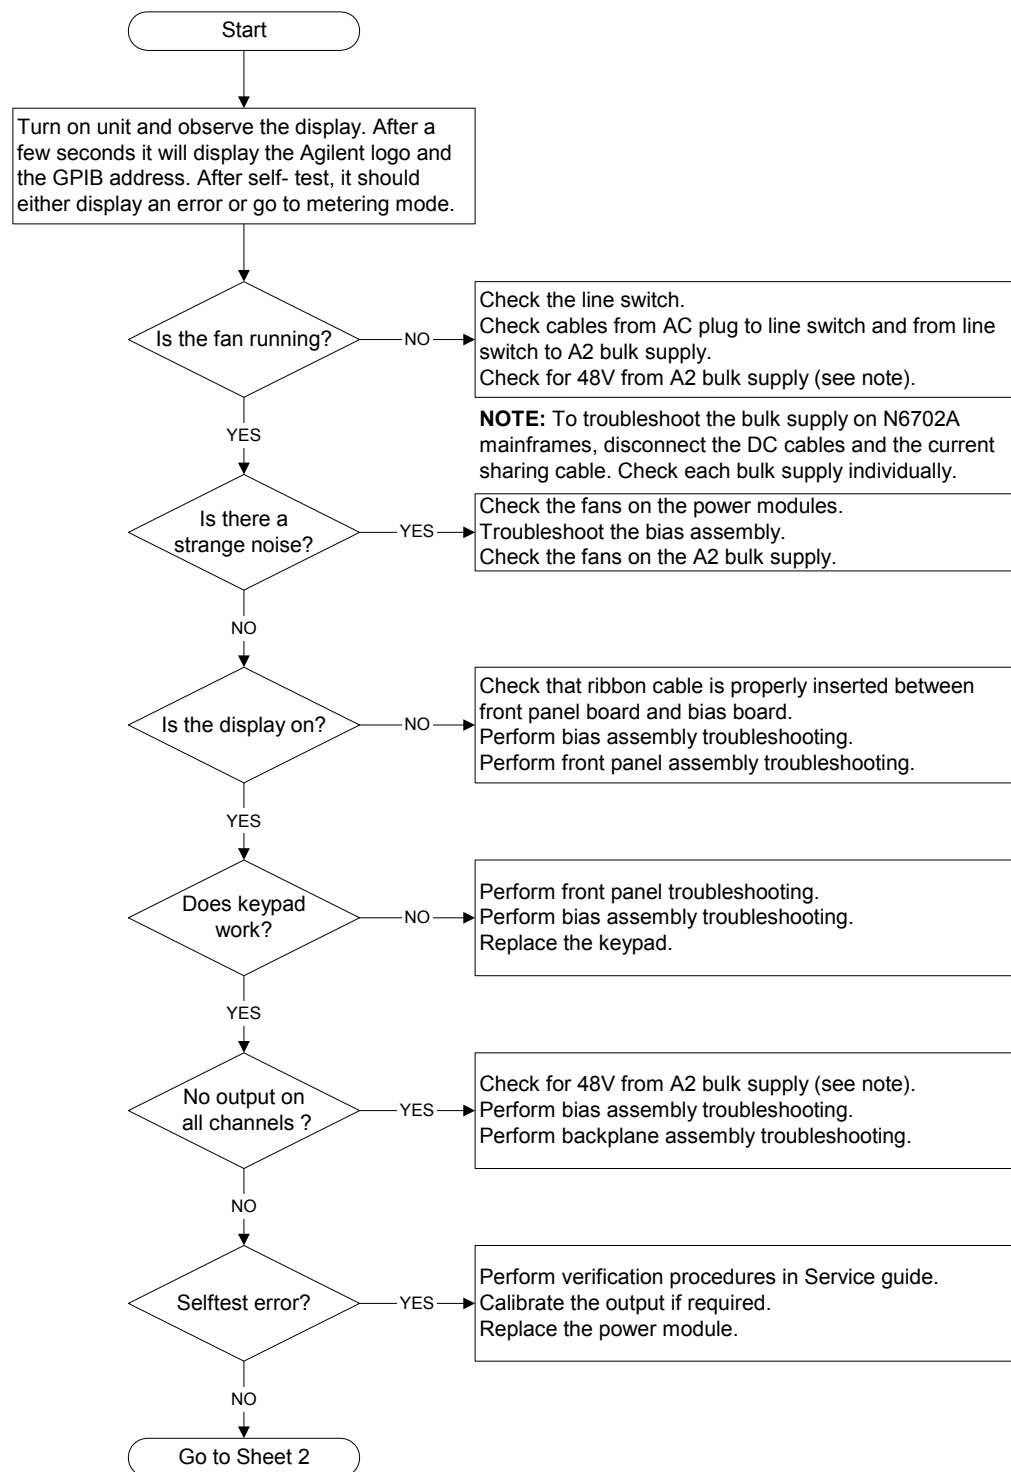


Figure 3-1. Overall Troubleshooting Sheet 1

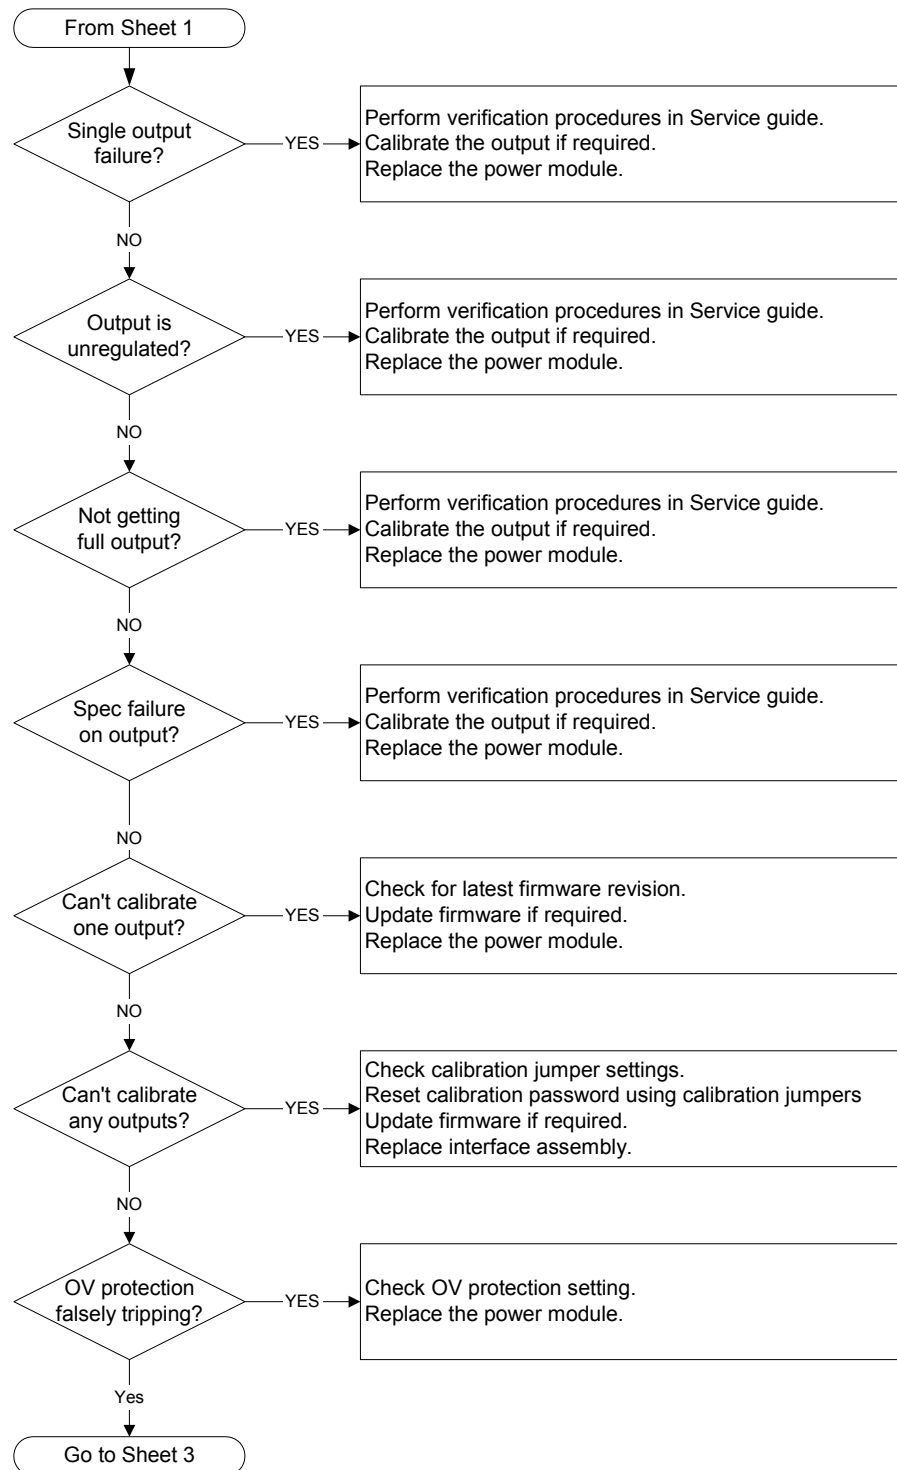


Figure 3-1. Overall Troubleshooting Sheet 2


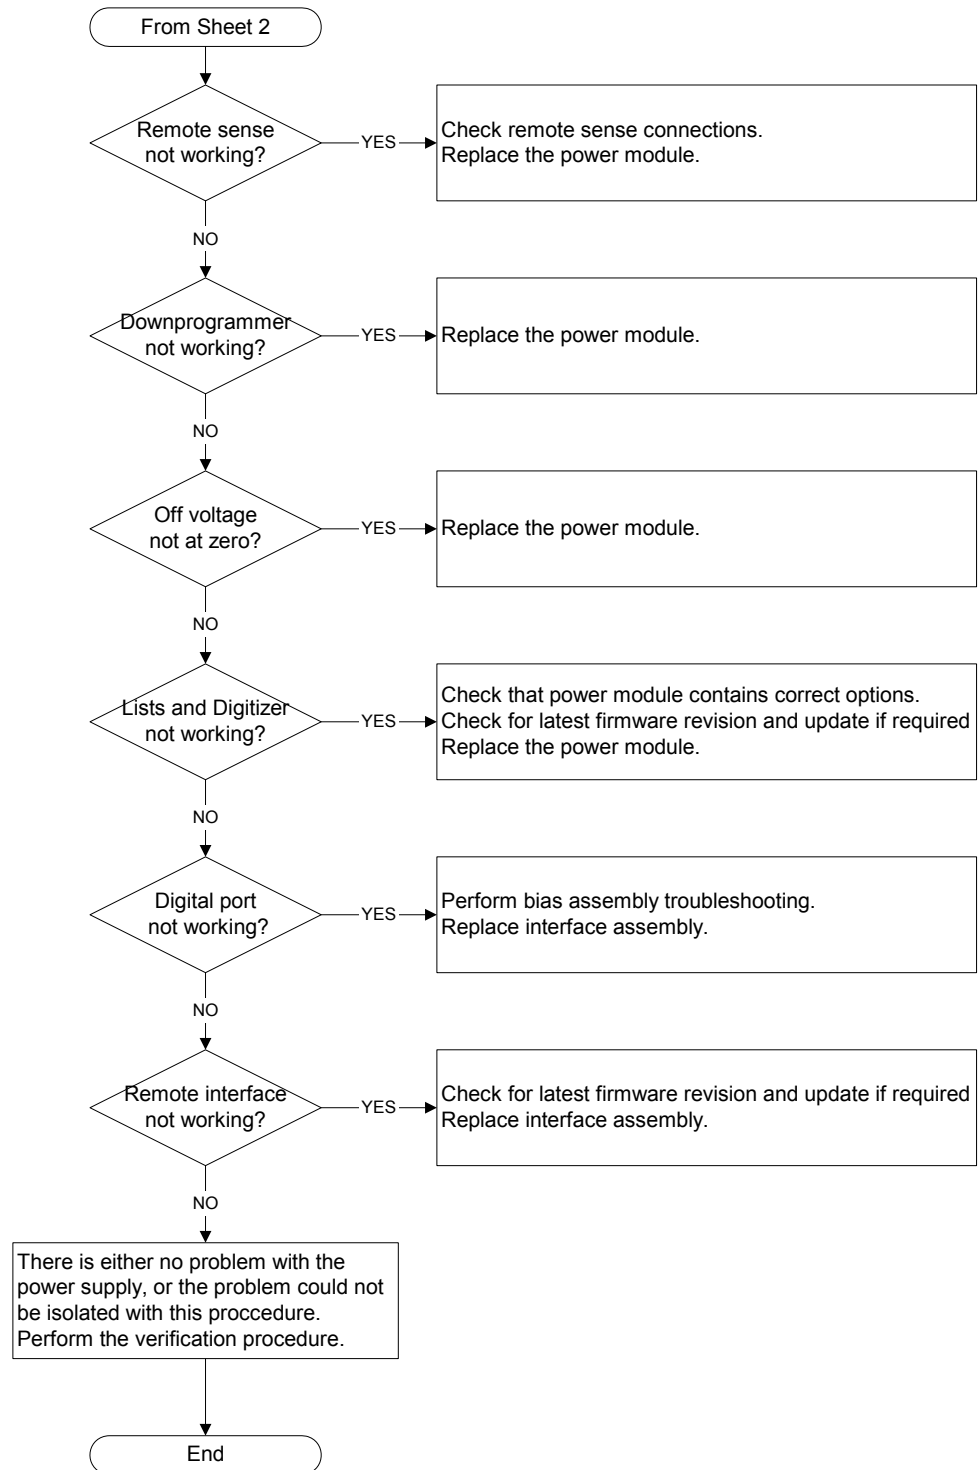


Figure 3-1. Overall Troubleshooting Sheet 3

Front Panel Troubleshooting

Troubleshooting the front panel board involves checking for the presence of the correct bias voltages on the board. Refer to the following table and figure.

Test Point	Location	Voltage	Action
TP 1	BKL_VCC	+12 V	If bias not present, troubleshoot the bias board or replace the front panel board.
TP 2	P1 pin 3	+12 V	If backlight voltage not present, replace the front panel board. If voltage is present and the display is not lit, replace the display.
Common	GNDB	Common	

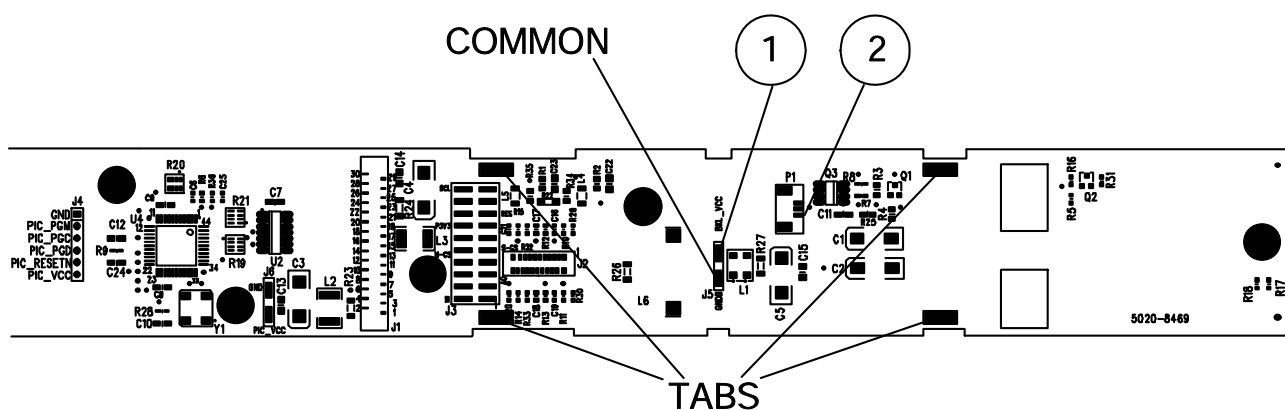


Bias Board Troubleshooting

Troubleshooting the bias board involves checking for the presence of the correct bias voltages on the board. Refer to the following table and figures.

Note that if the bias voltages at test points 2 - 4 in the following table are not present, it could be caused by a defect in the power module or interface board that is pulling the bias voltage low.

Test Point	Location	Voltage	Action
TP 1	+ RED	+48 V	Output of bulk supply. If not present, replace the bulk supply.
TP 2	+ C4	+12 V	If biases at TP 2, TP 3, or TP 4 are not present, disconnect the backplane and interface board cable assemblies and recheck. If biases are still not present, replace the bias board.
TP 3	U9 - 2	+5 V	Same as above.
TP 4	+ C3	+3.3 V	Same as above.
Common	- BLK	Common	

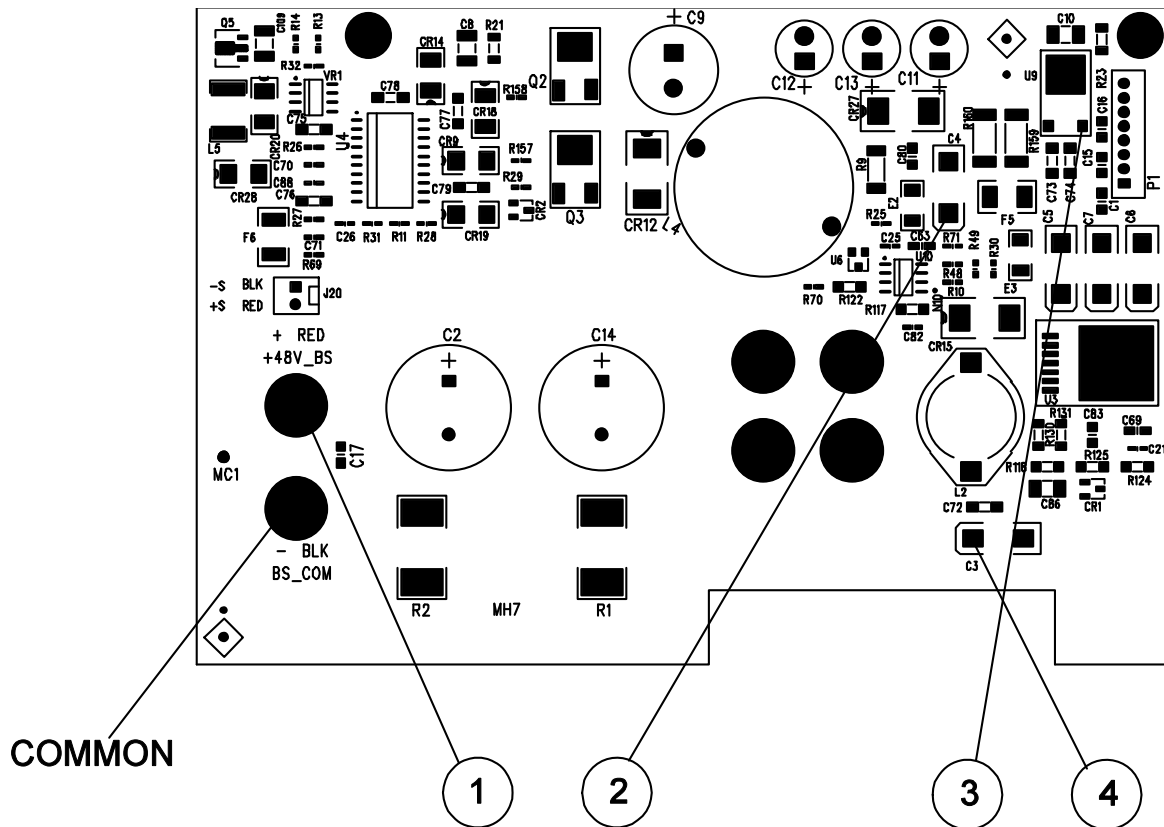

Backplane Board Troubleshooting

Troubleshooting the backplane board consists of visually inspecting the pins and pin connections.

If there are missing or broken pins, replace the board.

If there are bent pins, carefully try to straighten the pin. If you are unsuccessful, replace the board.

Closely examine the solder connections at the pins. If there are cracks in the solder, carefully re-solder the connector. If unsuccessful, replace the board.

Calibration and Passwords

Calibration is not required after the mainframe has been repaired. All calibration information is module-specific and resides in each power module.

However, if the A5 board that contains the calibration switches has been replaced, any calibration password that has been set will be lost. Passwords that are used to prevent access to the front panel Admin menu will also be lost.

The calibration password will automatically be reset to the factory default, which is zero (0). Front panel access to the Admin menu will be unrestricted unless a password is set.

Refer to the User's Guide for information on setting the calibration password as well as the Admin menu password.

Initialization

The power system's model number, serial number, and other constants that are required to program the instrument are stored in an EEPROM on the A5 board. If this board is replaced, the instrument must be re-initialized.

To initialize the power system, you must send the following information to the power system over the interface:


```
DIAGnostic:FRAMe:ATTRibute "ModelNumber", "value"
```

where "value" is the model number, e.g. N6700B.

```
DIAGnostic:FRAMe:ATTRibute "SerialNumber", "value"
```

where "value" is the serial number located on top of the interface cover.

At power-up, the power system will go through the turn-on self test sequence. All other parameters will be set to the factory defaults. The mainframe is now initialized.

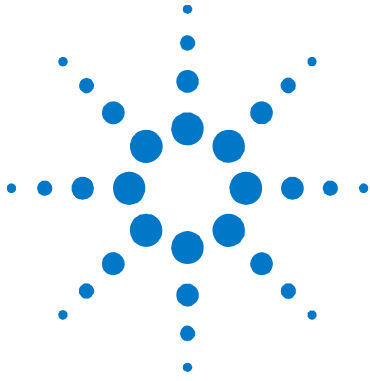

6

Replaceable Parts

Parts List	88
Parts Location Diagrams	89

The following table documents the replaceable parts assemblies. The diagrams show the location of the parts

Parts List

Reference Designator	N6700B Part number	N6701A Part number	N6702A Part number	Description
Electrical Assemblies				
A1	N6700-61001	N6700-61001	N6700-61001	A1 Front Panel PCA (tested)
A2	0950-4655	0950-4687	0950-4687 (qty. 2)	A2 Bulk Supply
A3	5065-6981	5065-6981	5065-6981	A3 Backplane PCA
A4	N6700-60101	N6700-60101	N6700-60101	A4 Bias PCA (tested)
A5	N6700-60102	N6700-60102	N6700-60102	A5 Interface PCA (tested)
Individual Parts				
1	5002-2817	5002-2817	5002-2828	Chassis frame
2	5002-2808	5002-2808	5002-2808	Front frame
3	1390-1079	1390-1079	1390-1079	Handles
4	N6700-40001	N6700-40001	N6700-40001	Keypad
5	2090-0886	2090-0886	2090-0886	Display
6	4040-2556	4040-2556	4040-2556	Window
7	N6700-00001	N6700-00001	N6700-00001	Front panel
8	3101-4019	3101-4019	3101-4019	Line switch
9	5185-1358	5185-1358	5185-1358 (qty. 2)	Cable, bulk supply to ground
10	5185-1357	5185-1357	5188-4205	AC cable, bulk supply to switch
11	5185-1362	5185-1362	5185-1362	DC power cable
12	5185-1354	5185-1354	5185-1354	Ribbon cable, to front panel
13	5185-1382	5185-1382	5185-1382	Ribbon cable, to backplane
14	5185-1352	5185-1352	5185-1352	Insulator, under backplane
15	5185-1384	5188-4210	5188-4210	Bias cable assembly
16	5185-1397	5185-1397	5185-1397	AC cable with socket
17	1510-0038	1510-0038	1510-0038	Binding post
18	E5810-61605	E5810-61605	E5810-61605	GPIO connector with cable
19	1253-6408	1253-6408	1253-6408	Digital plug
20	N.A.	5002-2830	N.A.	Bulk supply bracket
21	N.A.	N.A.	5188-4207	Current share cable
22	N.A.	N.A.	5188-4206	DC power cable for 2 nd bulk supply
Covers and Labels				
	5002-2809	5002-2809	5002-2829	Bulk supply cover
	5002-2810	5002-2810	5002-2810	Blower cover
	5002-2807	5002-2807	5002-2807	Interface cover
	N6700-80006	N6701-80006	N6702-80006	Front/Rear/Interface labels
	5185-1387	5185-1387	5185-1387	Blower cover label (caution)

Parts Location Diagrams

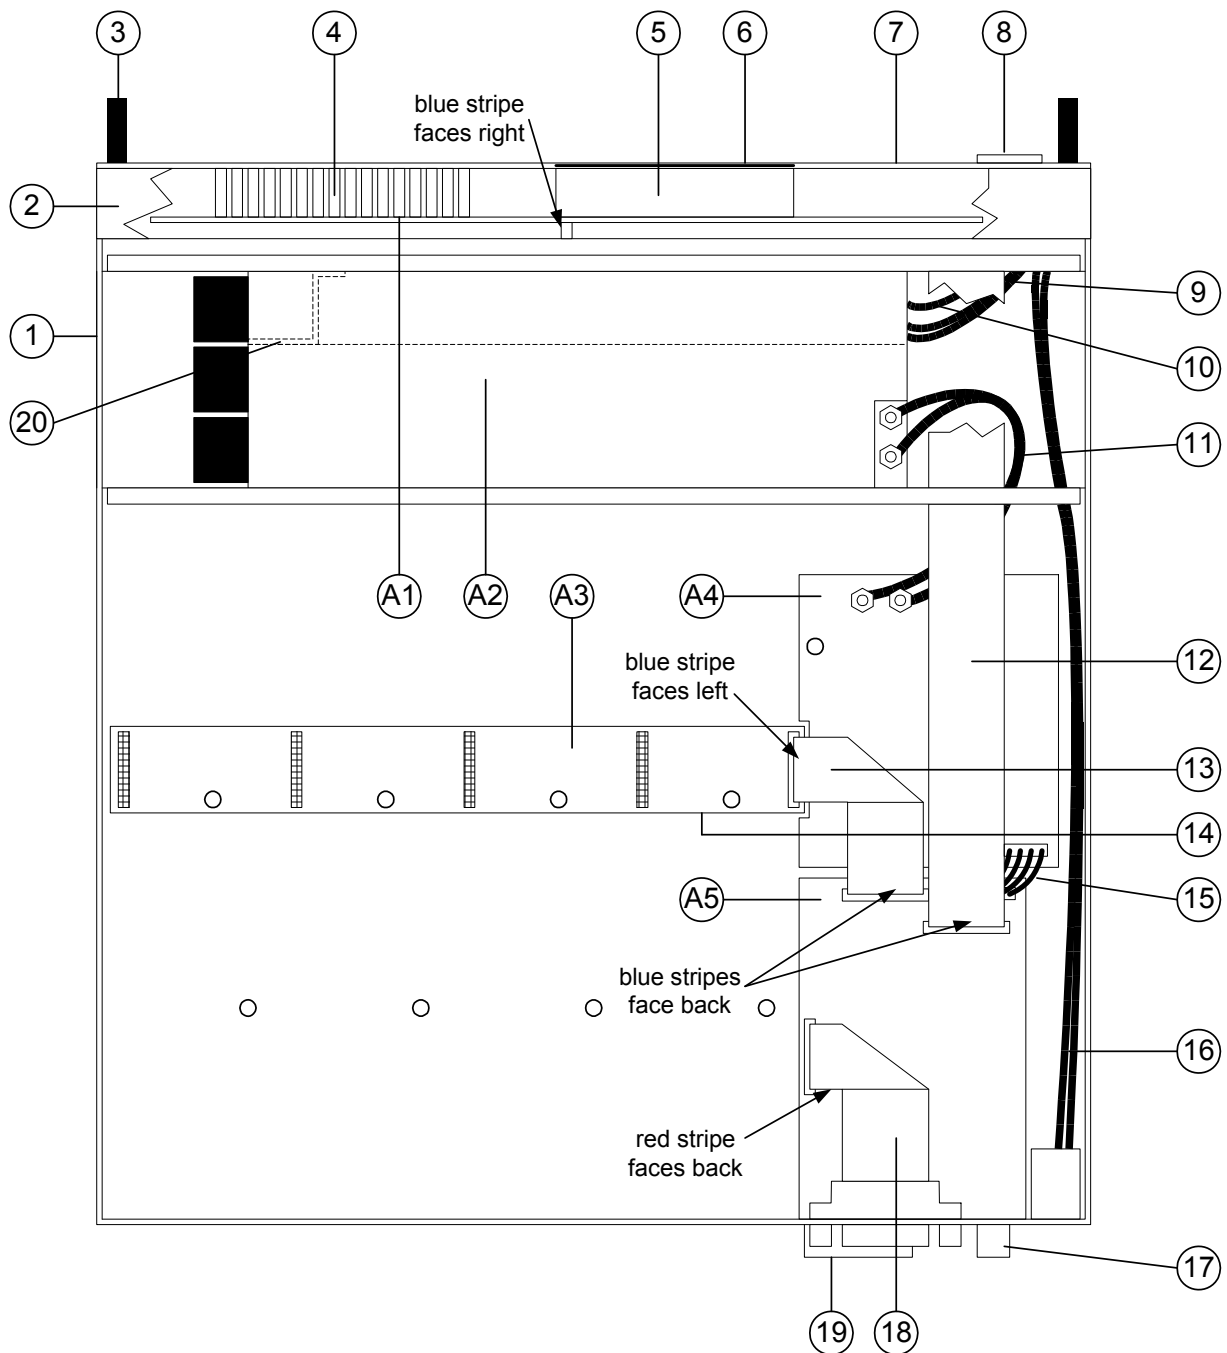


Figure 4-1. N6700B/N6701A Mainframe Part Locations


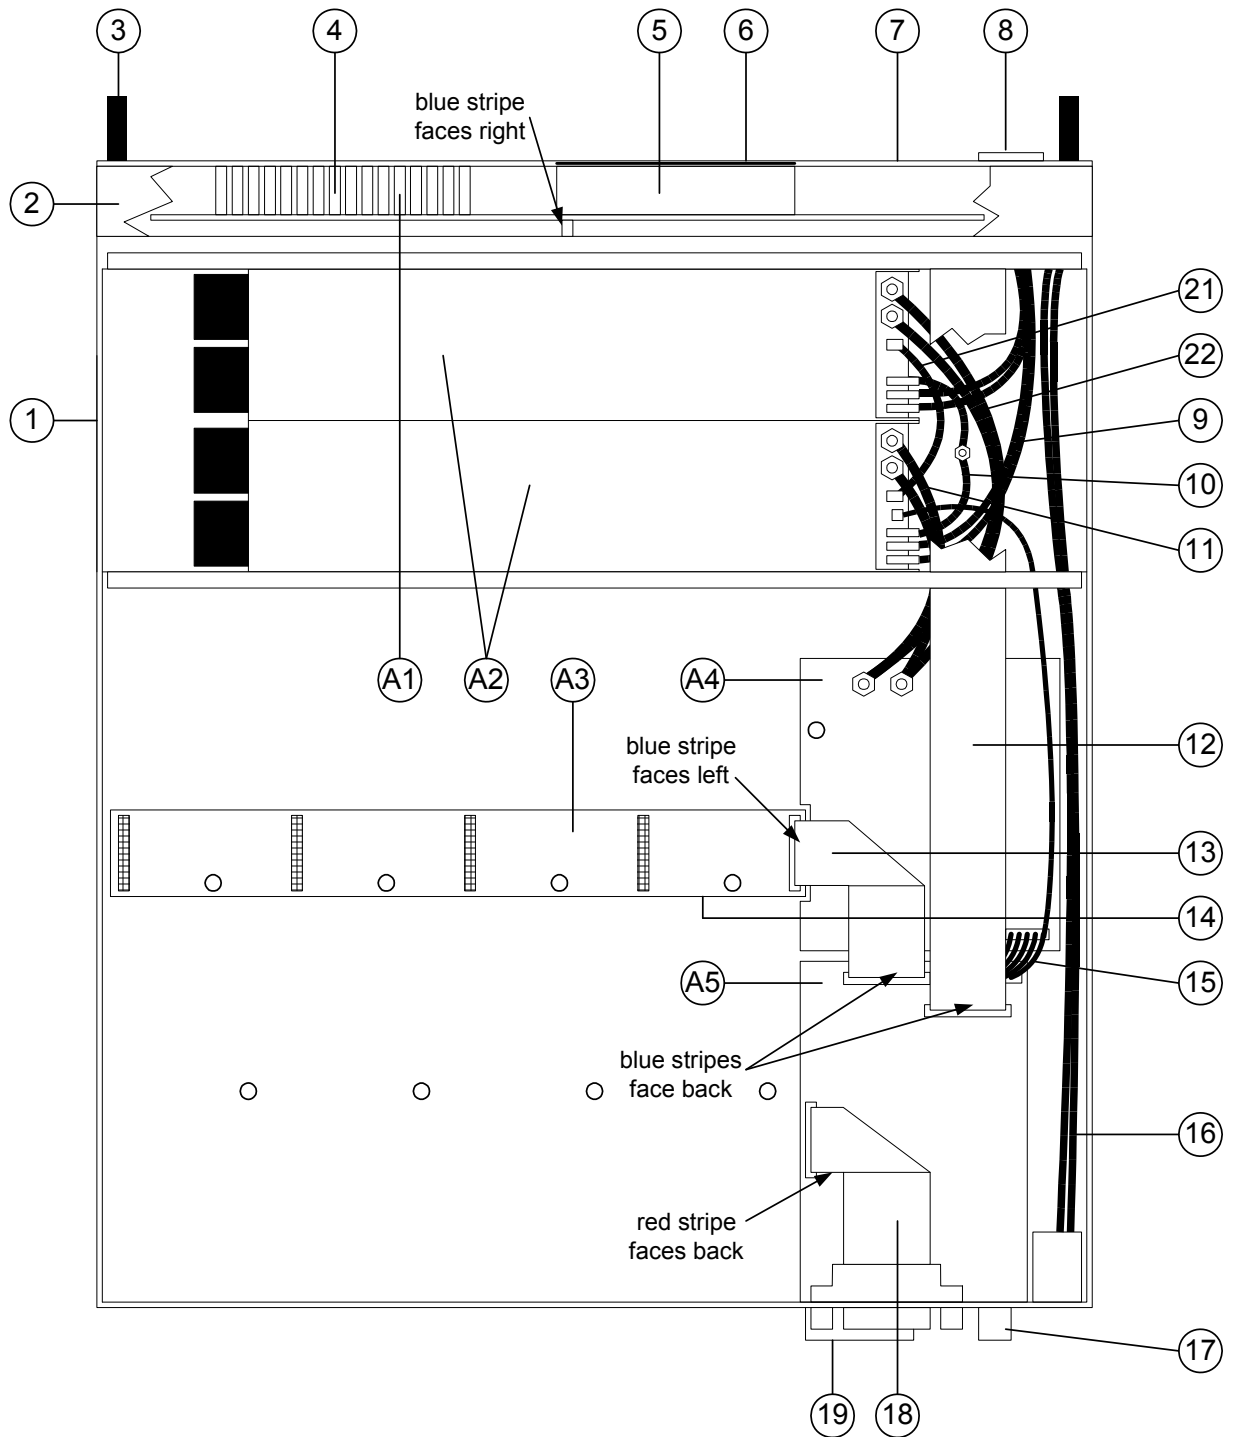


Figure 4-2. N6702A Mainframe Part Locations

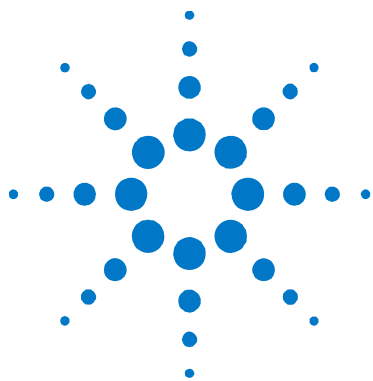

Appendix A

Error Messages

Displaying Error Messages	92
Error List	92

This appendix gives the error numbers and descriptions that are returned by the Agilent N6700 Modular Power System.

Error messages can be displayed on the front panel and also read back programmatically.

Displaying Error Messages

The instrument beeps each time a command syntax or hardware error is generated. The front-panel **ERR** annunciator turns on when one or more errors are currently stored in the SCPI error queue.

Front Panel:	SCPI Command:
Press the Error key.	SYST : ERR?
If errors appear, use the navigation keys to scroll through the list.	

Errors are cleared as they are read. When all errors have been read, the **ERR** annunciator turns off and the error queue is cleared.

Error List


Error	Device-dependent Errors (these errors set Standard Event Status register bit #3)
0	No error This is the response to the ERR? query when there are no errors.
100	Too many channels You have specified more channels than are installed in the mainframe.
101	Calibration state is off Calibration is not enabled. The instrument will not accept calibration commands.
102	Calibration password is incorrect The calibration password is incorrect.
103	Calibration is inhibited by switch setting Calibration mode is locked out by the calibration switch.
104	Bad sequence of calibration commands Calibration commands have not been entered in the proper sequence.
105	Unexpected output current The measured output current is outside the acceptable range.
106	Zero measurement out of range error The "zero" measurement value is outside the acceptable range.
107	Programming cal constants out of range The programmed calibration constant is outside the acceptable range.
108	Measurement cal constants out of range The measurement calibration constant is outside the acceptable range.
109	Over voltage cal constants out of range The over voltage calibration constant is outside the acceptable range.
110	Wrong V+I The instrument was unable to set the correct voltage or current value.
111	Aux vloc cal constants out of range Calibration constants on the internal auxiliary local ADC are outside the acceptable range.
112	Aux vrem cal constants out of range Calibration constants on the internal auxiliary remote ADC are outside the acceptable range.
113	Aux imon cal constants out of range Calibration constants on the internal auxiliary imon ADC are outside the acceptable range.

Device-dependent Errors (continued)	
200	Hardware error channel <channel> A hardware error has occurred on the specified channel.
201	Invalid configuration, empty slots There is an empty slot between modules. This configuration is not allowed.
202	Selftest Fail A selftest failure has occurred. See selftest failure list for details.
203	Compatibility function not implemented The requested compatibility function is not available.
204	NVRAM checksum error A checksum error has occurred in the instrument's nonvolatile random access memory.
205	NVRAM full The nonvolatile random access memory of the instrument is full.
206	File not found The internal calibration file or the internal channel attribute file was not found in NVRAM.
207	Cal file version error The calibration file was written or read using old firmware. Firmware must be updated.
302	Option not installed The option that is programmed by this command is not installed.
303	There is not a valid acquisition to fetch from There is no valid data in the measurement buffer.
304	Volt and curr in incompatible transient modes Voltage and current cannot be in Step and List mode at the same time.
305	A triggered value is on a different range A triggered value is on a different range than the one that is presently set.
306	Too many list points Too many list points have been specified.
307	List lengths are not equivalent One or more lists are not the same length.
308	This setting cannot be changed while transient trigger is initiated Setting cannot be changed while the instrument is waiting for or executing a trigger sequence.
309	Cannot initiate, voltage and current in fixed mode Cannot initiate the transient generator because either the voltage or the current function is set to Fixed mode.
Command Errors (these errors set Standard Event Status register bit #5)	
-100	Command error Generic syntax error.
-101	Invalid character An invalid character was found in the command string.
-102	Syntax error Invalid syntax was found in the command string. Check for blank spaces.
-103	Invalid separator An invalid separator was found in the command string. Check for proper use of , ; :
-104	Data type error A different data type than the one allowed was found in the command string.
-105	GET not allowed A group execute trigger is not allowed in a command string.

Command Errors (continued)	
–108	Parameter not allowed More parameters were received than were expected.
–109	Missing parameter Fewer parameters were received than were expected.
–110	Command header error An error was detected in the header.
–111	Header separator error A character that was not a valid header separator was found in the command string.
–112	Program mnemonic too long The header contains more than 12 characters.
–113	Undefined header A command was received that was not valid for this instrument.
–114	Header suffix out of range The value of the numeric suffix is not valid.
–120	Numeric data error Generic numeric data error.
–121	Invalid character in number An invalid character for the data type was found in the command string.
–123	Exponent too large The magnitude of the exponent was larger than 32000.
–124	Too many digits The mantissa of a numeric parameter contained more than 255 digits, excluding leading zeros.
–128	Numeric data not allowed A numeric parameter was received but a character string was expected.
–130	Suffix error Generic suffix error
–131	Invalid suffix A suffix was incorrectly specified for a numeric parameter.
–134	Suffix too long The suffix contains more than 12 characters.
–138	Suffix not allowed A suffix is not supported for this command.
–140	Character data error Generic character data error
–141	Invalid character data Either the character data element contains an invalid character, or the element is not valid.
–144	Character data too long The character data element contains more than 12 characters.
–148	Character data not allowed A discrete parameter was received, but a string or numeric parameter was expected.
–150	String data error Generic string data error
–151	Invalid string data An invalid character string was received. Check that the string is enclosed in quotation marks.
–158	String data not allowed A character string was received, but is not allowed for this command.

Command Errors (continued)	
–160	Block data error Generic block data error
–161	Invalid block data The number of data bytes sent does not match the number of bytes specified in the header.
–168	Block data not allowed Data was sent in arbitrary block format but is not allowed for this command.
–170	Expression error Generic expression error
–171	Invalid expression data The expression data element was invalid.
–178	Expression data not allowed Expression data element was sent but is not allowed for this command.
Execution Errors (these errors set Standard Event Status register bit #4)	
–200	Execution error Generic syntax error
–220	Parameter error A data element related error occurred.
–221	Settings conflict A data element could not be executed because of the present instrument state.
–222	Data out of range A data element could not be executed because the value was outside the valid range.
–223	Too much data A data element was received that contains more data than the instrument can handle.
–224	Illegal parameter value An exact value was expected but not received.
–225	Out of memory The device has insufficient memory to perform the requested operation.
–226	Lists not same length One or more lists are not the same length.
–230	Data corrupt or stale Possible invalid data. A new reading was started but not completed.
–231	Data questionable The measurement accuracy is suspect.
–232	Invalid format The data format or structure is inappropriate.
–233	Invalid version The version of the data format is incorrect to the instrument.
–240	Hardware error The command could not be executed because of a hardware problem with the instrument.
–241	Hardware missing The command could not be executed because of missing hardware, such as an option.
–260	Expression error An expression program data element related error occurred.
–261	Math error in expression An expression program data element could not be executed due to a math error.

Query Errors (these errors set Standard Event Status register bit #2)	
-400	Query Error Generic error query
-410	Query INTERRUPTED A condition causing an interrupted query error occurred.
-420	Query UNTERMINATED A condition causing an unterminated query error occurred.
-430	Query DEADLOCKED A condition causing a deadlocked query error occurred.
-440	Query UNTERMINATED after indefinite response A query was received in the same program message after a query indicating an indefinite response was executed.
Selftest Errors (these errors set Standard Event Status register bit #3)	
202	Selftest Fail Aux Adc 0 expected <n1> to <n2>, measured <n3>, chan <n4> Auxiliary ADC failed. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 0 expected <n1> to <n2>, measured <n3>, chan <n4> Both voltage and current DACs are at zero. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 1 expected <n1> to <n2>, measured <n3>, chan <n4> Voltage DAC is at zero; current DAC is at full scale. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 2 expected <n1> to <n2>, measured <n3>, chan <n4> Voltage DAC is at full scale; current DAC is at zero. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.
202	Selftest Fail DACs 3 expected <n1> to <n2>, measured <n3>, chan <n4> Both voltage and current DACs are at full scale. n1 and n2 are the expected limits. n3 is the measured value. n4 is the channel location of the failed module.

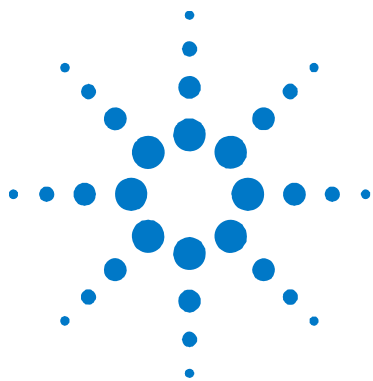

Appendix B Backdating

Firmware Differences	98
--	----

This appendix discusses differences in firmware revisions prior to revision D.00.00 and C.00.00.

Firmware Differences

Firmware Revisions Prior to D.00.00

The following features and capabilities are **not** available on mainframes with firmware revisions prior to D.00.00.

- Support for the Agilent N678xA power modules.

Firmware Revisions Prior to C.00.00

The following features and capabilities are **not** available on mainframes with firmware revisions prior to C.00.00.

- Support for the 300 W power modules.
- The power allocation function for power modules.
- The ability to reverse the polarity of the output and sense connectors.
- Compliance with LXI class C.

NOTE

To upgrade your instrument with the latest firmware revision, go to <http://www.agilent.com/find/N6700firmware>.

Front Panel Menu Commands for Firmware Revisions prior to D.00.00

Menu Command				Control Description		
Output	Voltage		Programs voltage setting and range.			
	Current		Programs current setting and range.			
	Delay		Programs Turn-on /Turn off delay.			
	Slew		Programs voltage slew rate.			
	Power		Programs the power allocation function.			
	Pol		Lets you reverse the polarity of the output and sense terminals.			
	Couple		Couples output channels for output on/off synchronization.			
Measure	Range		Selects voltage and current measurement range.			
	Sweep		Specifies measurement points, time interval, and trigger offset.			
	Window		Selects measurement window: Rectangular, Hanning.			
	Control		Lets you abort a measurement in progress.			
Transient	Mode		Selects voltage or current transient mode: Fixed, Step, List.			
	Step		Programs voltage and current step value. Enables step triggers.			
	List	Pace		Specifies Dwell or Trigger paced list.		
		Repeat		Specifies number of list repetitions, or specifies continuous list.		
		Terminate		Specifies list settings when the list terminates.		
		Config		Configures list step voltage, current, dwell, and trigger signals.		
		Reset		Aborts the list and resets all list parameters.		
	TrigSource		Specify the trigger source: Bus, Tran 1-4, Pin 1-7.			
	Control		Initiates, Triggers, or Aborts output triggers. Displays trigger state.			
Protect	OVP		Configures over-voltage protection function.			
	OCP		Configures over-current protection function.			
	Inhibit		Configures the external inhibit signal: Off, Latching, Live			
	Coupling		Disables ALL output channels when a protection fault occurs.			
	Clear		Clears output protection. Displays output state.			
States	Reset		Resets the instrument to its reset (*RST) state.			
	SaveRecall		Saves or recalls an instrument state.			
	PowerOn		Selects the power-on state: *RST, RCL0.			
System	IO	LAN	ActiveSettings		Displays the LAN interface settings that are presently active.	
			Config	IP	Configures the IP addressing of the instrument.	
				Name	Configures the Dynamic DNS and NetBIOS naming service.	
				Domain	Configures the Domain Name.	
				DNS	Configures the DNS server.	
				TCP	Configures the TCP keepalive function.	
				Reset	Resets the LAN interface settings to the factory-shipped state.	
		USB	Status	Displays status, speed, packets received, and packets sent.		
			Identification	USB connect string - the instrument’s unique USB identifier.		
			GPIB	Selects the GPIB address.		

Menu Command				Control Description	
System	IO	DigPort	Pin1	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut, FaultOut. Specifies the pin polarity: Positive, Negative
			Pin2	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut. Specifies the pin polarity: Positive, Negative
			Pin3	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut, InhibitIn. Specifies the pin polarity: Positive, Negative
			Pin4	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut, OnC, OffC. Specifies the pin polarity: Positive, Negative
			Pin5	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut, OnC, OffC. Specifies the pin polarity: Positive, Negative
			Pin6	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut, OnC, OffC. Specifies the pin polarity: Positive, Negative
			Pin7	Function Polarity	Specifies the pin function: DigIn, DigIO, TrigIn, TrigOut, OnC, OffC. Specifies the pin polarity: Positive, Negative
			Data		Sends/reads data from the digital I/O port
Groups				Defines groups of output channels that are connected in parallel.	
Preferences	Display	Contrast		Configures the display contrast.	
		Saver		Configures the screen saver and wake-on I/O timer.	
		View		Selects 1-channel or 4-channel view at turn-on	
		Keys		Enables/disables key clicks and configures the On/Off key.	
		Lock		Locks front panel keys. Enter a password to unlock the front panel.	
Admin	Login/Logout		Enter a password to access the admin functions.		
	Cal	Function	Vprog	High	Enters measured data for the High calibration point.
				Low	Enters measured data for the Low calibration point.
			Vmeas	Enters measured data.	
			CMRR	Calibrates common mode rejection ratio.	
			Iprog	High	Enters measured data for the High calibration point.
				Low	Enters measured data for the Low calibration point.
			Imeas	100mA	Enters measured data for the 100 mA range point.
				200uA	Enters measured data for the 200 μA range point.
			Dprog	Calibrates the downprogrammer.	
			Ipeak	Calibrates I peak.	
			Date	Saves the calibration date for each channel.	
			Save	Saves the calibration data.	
	LAN		Enables/disables the LAN interface and the built-in Web server.		
	USB		Enables/disables the USB interface.		
	Nvram		Resets all non-volatile RAM settings to their factory defaults.		
	Password		Changes the password for the admin functions.		
About	Frame		Displays model, serial number, and firmware revisions.		
	Module		Displays model, serial number, options, voltage, current, power.		

Front Panel Menu Commands for Firmware Revisions prior to C.00.00

Menu Command			Control Description	
Output	Voltage		Programs voltage setting and range.	
	Current		Programs current setting and range.	
	Delay		Program Turn-on /Turn Off delay.	
Measure	Range		Selects voltage and current measurement range.	
	Sweep		Specifies measurement points, time interval, and trigger offset.	
	Window		Selects measurement window (Rectangular/Hanning).	
	Control		Lets you abort a measurement in progress.	
Transient	Mode	Voltage	Selects voltage mode (Fixed, Step, or List).	
		Current	Selects current mode (Fixed, Step, or List).	
	Step		Programs voltage and current steps. Enables step trigger signals.	
	List	Pace	Specifies Dwell or Trigger paced list.	
		Repeat	Specifies number of list repetitions, or specifies continuous list.	
		Terminate	Specifies list settings when the list terminates.	
		Config	Configures the list steps. Specify voltage, current, and dwell values. Also specifies trigger output signal states.	
	Reset		Aborts the list and resets all list parameters.	
	TrigSource		Specify the trigger source: bus, tran 1-4, pin 1-3.	
	Control		Initiate, Trigger, or Abort output triggers.	
Protect	OVP		Configures over-voltage protections function.	
	OCP		Configures over-current protections function.	
	Inhibit		Configures the external inhibit signal.	
	Coupling		Disables ALL output channels when a protection fault occurs.	
	Clear		Clears output protection.	
States	Reset		Resets the instrument to its reset (*RST) state.	
	Save/Recall		Saves or recalls an instrument state.	
	PowerOn		Selects the power on state.	
System	Interface	LAN	Status	Displays interface status information.
			IP	Enables/disables DHCP and Auto IP
				Also sets the IP Address, Subnet Mask, and Default Gateway.
			DNS	Configures the DNS server.
			Name	Configures the Dynamic DNS and NetBIOS naming service.
			Domain	Configures the Domain Name.
			TCP	Configures the TCP keepalive function.
		Enable	Enables/disables the LAN interface and the built-in Web server.	
		USB	Status	Displays status, speed, packets received, and packets sent.
			Identification	USB connect string - the instrument’s unique USB identifier
			Enable	Enables/disables the USB interface.
		GPIB		Selects the GPIB address.
		Reset		Resets the interface settings to the factory-shipped state.

Menu Command				Control Description	
System	DigPort	Pin 1	Function	Specifies the pin function: DigIO, TrigIn, TrigOut, DigIn, or FaultOut..	
			Polarity	Specifies the pin polarity.	
Pin 2		Function	Specifies the pin function: DigIO, TrigIn, TrigOut, or DigIn.		
		Polarity	Specifies the pin polarity.		
Pin 3		Function	Specifies the pin function: DigIO, TrigIn, TrigOut, DigIn, or InhibitIn.		
		Polarity	Specifies the pin polarity.		
Data		Sends/reads data from the digital I/O port function			
Preferences		Display		Configures Screen saver, Wake-on I/O, and Display contrast.	
		Keys		Enables/disables key clicks and configures the On/Off key.	
		Security	ResetNVRam	Resets all non-volatile RAM settings to their factory defaults.	
Error				Displays the Error log.	
Calibrate	State		Enables/disables calibration. You must supply a password to enable.		
	Sequence	VProg	High	Enters measured data for high calibration point.	
			Low	Enters measured data for low calibration point.	
		VMeas		Enters measured data.	
		CMRR		Calibrates common mode rejection ratio.	
		IProg	High	Enters measured data for high calibration point.	
			Low	Enters measured data for low calibration point.	
		IMeas		Enters Measured data.	
		DPRog		Calibrates the downprogrammer.	
	IPeak		Calibrates I peak.		
	Date		Saves the calibration date for each channel.		
	Save		Saves the calibration data.		
	Password		Changes the password.		
	About	Frame		Displays model, serial number, firmware revision, backup revision, and active firmware.	
Module		Displays model, serial number, options, voltage, current, and power.			

Index

A	
assemblies	
replaceable.....	58
B	
backplane board	55
bias board	45, 54
bulk supply.....	46
C	
calibration	32
current downprogrammer	37
current programming and measurement.....	36
enable	31, 33
equipment	10
low range current measurement	37, 71
low range current programming	38
low range voltage measurement	35
low range voltage programming	34
password	40
peak current limit.....	39
post repair	56
save and exit.....	40
switches	32, 44
voltage common mode rejection	35
voltage programming and measurement	33
Caution	3
CC	
load effect	16
source effect.....	17
contact numbers.....	5
current	
monitoring resistor	11
programming accuracy	15
readback accuracy.....	15
CV	
load effect	12
noise.....	13
source effect.....	13
D	
differences in N6700A mainframes	68
disassembly	42, 43
bias board.....	45

bulk supply	46
front panel	45
interface board.....	45
parts location	59
ribbon cables.....	42
tools	42
E	
electronic load.....	11
electrostatic discharge precautions	6, 42
error codes	62
displaying.....	62
selftest	50
F	
firmware upgrade.....	7
flowchart	51
front panel.....	45, 54
menus.....	69
G	
ground	
redundant for 400 Hz	47
H	
history	2
I	
initialization	
post repair	56
installing modules	43
instrument	
identification	6, 7
interface board	45
O	
operating checklist.....	6
overall troubleshooting.....	51
P	
password	
calibration.....	32
post repair	56

Index

T

transient recovery time 14

	W	
Warning.....		3
Web URL's.....		5, 7